

FIASP- insulin aspart injection injection, solution

Novo Nordisk

HIGHLIGHTS OF PRESCRIBING INFORMATION

These highlights do not include all the information needed to use FIASP safely and effectively. See full prescribing information for FIASP.

FIASP® (insulin aspart) injection, for subcutaneous or intravenous use
Initial U.S. Approval: 2000

INDICATIONS AND USAGE

- FIASP is a rapid-acting human insulin analog indicated to improve glycemic control in adult and pediatric patients with diabetes mellitus (1).

DOSAGE AND ADMINISTRATION

- Individualize and adjust the dosage of FIASP based on route of administration, individual's metabolic needs, blood glucose monitoring results and glycemic control goal (2.3).
- Dosage adjustments may be needed when switching from another insulin, with changes in physical activity, changes in concomitant medications, changes in meal patterns, changes in renal or hepatic function or during acute illness (2.3).
- *Subcutaneous injection (2.2):*
 - Inject at the start of a meal or within 20 minutes after starting a meal into the abdomen, upper arm, or thigh.
 - Rotate injection sites within the same region to reduce the risk of lipodystrophy and localized cutaneous amyloidosis.
 - Should generally be used in regimens with an intermediate- or long-acting insulin.
- *Continuous Subcutaneous Infusion (Insulin Pump) (2.2):*
 - Refer to the insulin infusion pump user manual to see if FIASP can be used. Use in accordance with the insulin pumps' instructions for use.
 - Administer by continuous subcutaneous infusion using an insulin pump in a region recommended in the instructions from the pump manufacturer. Rotate infusion sites within the same region to reduce the risk of lipodystrophy and localized cutaneous amyloidosis.
- *Intravenous Infusion:* Administer only under medical supervision after diluting to concentrations from 0.5 to 1 unit/mL insulin aspart in infusion systems using polypropylene infusion bags (2.2).

DOSAGE FORMS AND STRENGTHS

Injection: 100 units/mL (U-100) available as:

- 10 mL multiple-dose vial (3)
- 3 mL single-patient-use FIASP FlexTouch® pen (3)
- 3 mL single-patient-use PenFill® cartridges for use in a PenFill cartridge device (3)
- 1.6 mL single-patient-use PumpCart® cartridges for use in a compatible insulin pump (3)

CONTRAINDICATIONS

- During episodes of hypoglycemia (4).
- Hypersensitivity to insulin aspart or any of the excipients in FIASP (4).

WARNINGS AND PRECAUTIONS

- *Never share* a FIASP FlexTouch pen, PenFill cartridge or PenFill cartridge device between patients, even if the needle is changed (5.1).
- *Hyperglycemia or hypoglycemia with changes in insulin regimen:* Make changes to a patient's insulin regimen (e.g., insulin strength, manufacturer, type, injection site or method of administration) under close medical supervision with increased frequency of blood glucose monitoring (5.2).
- *Hypoglycemia:* May be life-threatening. Increase frequency of glucose monitoring with changes to: insulin dosage, co-administered glucose lowering medications, meal pattern, physical activity; and in

- patients with renal impairment or hepatic impairment or hypoglycemia unawareness (5.3).
- *Hypoglycemia due to medication errors*: Accidental mix-ups between insulin products can occur. Instruct patients to check insulin labels before injection (5.4).
 - *Hypokalemia*: May be life-threatening. Monitor potassium levels in patients at risk for hypokalemia and treat if indicated (5.5).
 - *Hypersensitivity reactions*: Severe, life-threatening, generalized allergy, including anaphylaxis, can occur. Discontinue FIASP, monitor and treat if indicated (5.6).
 - *Fluid retention and heart failure with concomitant use of thiazolidinediones (TZDs)*: Observe for signs and symptoms of heart failure; consider dosage reduction or discontinuation if heart failure occurs (5.7).
 - *Hyperglycemia and Ketoacidosis Due to Insulin Pump Device Malfunction*: Monitor glucose and administer FIASP by subcutaneous injection if pump malfunction occurs (5.8).

----- **ADVERSE REACTIONS** -----

Adverse reactions observed with FIASP include: hypoglycemia, allergic reactions, hypersensitivity, injection/infusion site reactions, lipodystrophy, and weight gain (6.1).

To report SUSPECTED ADVERSE REACTIONS, contact Novo Nordisk Inc. at 1-800-727-6500 or FDA at 1-800-FDA-1088 or www.fda.gov/medwatch.

----- **DRUG INTERACTIONS** -----

- *Drugs that Increase Hypoglycemia Risk or Increase or Decrease Blood Glucose Lowering Effect*: Adjustment of dosage may be needed; closely monitor blood glucose (7).
- *Drugs that Blunt Hypoglycemia Signs and Symptoms (e.g., beta-blockers, clonidine, guanethidine, and reserpine)*: Increased frequency of glucose monitoring may be required (7).

See 17 for PATIENT COUNSELING INFORMATION and FDA-approved patient labeling.

Revised: 6/2023

FULL PRESCRIBING INFORMATION: CONTENTS*

1 INDICATIONS AND USAGE

2 DOSAGE AND ADMINISTRATION

2.1 Important Preparation and Administration Instructions

2.2 Route of Administration Instructions

2.3 Dosage Recommendations

3 DOSAGE FORMS AND STRENGTHS

4 CONTRAINDICATIONS

5 WARNINGS AND PRECAUTIONS

5.1 Never Share a FIASP FlexTouch Pen, PenFill Cartridge or PenFill Cartridge Device Between Patients

5.2 Hyperglycemia or Hypoglycemia with Changes in Insulin Regimen

5.3 Hypoglycemia

5.4 Hypoglycemia Due to Medication Errors

5.5 Hypokalemia

5.6 Hypersensitivity and Allergic Reactions

5.7 Fluid Retention and Heart Failure with Concomitant Use of PPAR-Gamma Agonists

5.8 Hyperglycemia and Ketoacidosis Due to Insulin Pump Device Malfunction

6 ADVERSE REACTIONS

6.1 Clinical Trial Experience

6.2 Postmarketing Experience

7 DRUG INTERACTIONS

8 USE IN SPECIFIC POPULATIONS

8.1 Pregnancy

- 8.2 Lactation
- 8.4 Pediatric Use
- 8.5 Geriatric Use
- 8.6 Renal Impairment
- 8.7 Hepatic Impairment

10 OVERDOSAGE

11 DESCRIPTION

12 CLINICAL PHARMACOLOGY

- 12.1 Mechanism of Action
- 12.2 Pharmacodynamics
- 12.3 Pharmacokinetics
- 12.6 Immunogenicity

13 NONCLINICAL TOXICOLOGY

- 13.1 Carcinogenesis, Mutagenesis, Impairment of Fertility

14 CLINICAL STUDIES

- 14.1 Overview of Clinical Studies
- 14.2 Type 1 Diabetes Mellitus - Adults
- 14.3 Type 1 Diabetes Mellitus - Pediatric Patients
- 14.4 Type 2 Diabetes Mellitus - Adults
- 14.5 Type 1 Diabetes Mellitus- Adult Continuous Subcutaneous Insulin Infusion (CSII)

16 HOW SUPPLIED/STORAGE AND HANDLING

- 16.1 How Supplied
- 16.2 Recommended Storage

17 PATIENT COUNSELING INFORMATION

INSTRUCTIONS FOR USE
INSTRUCTIONS FOR USE
INSTRUCTIONS FOR USE
INSTRUCTIONS FOR USE

* Sections or subsections omitted from the full prescribing information are not listed.

FULL PRESCRIBING INFORMATION

1 INDICATIONS AND USAGE

FIASP is indicated to improve glycemic control in adult and pediatric patients with diabetes mellitus.

2 DOSAGE AND ADMINISTRATION

2.1 Important Preparation and Administration Instructions

- Always check insulin label before administration [*see Warnings and Precautions (5.4)*].
- Inspect FIASP visually before use. It should appear clear and colorless. Do not use FIASP if particulate matter or coloration is seen.
- Use FIASP FlexTouch pen with caution in patients with visual impairment who may

- rely on audible clicks to dial their dose.
- Use PenFill cartridges with caution in patients with visual impairment.
- Do **not** mix FIASP with any other insulin.

2.2 Route of Administration Instructions

Subcutaneous Injection:

- Inject FIASP at the start of a meal or within 20 minutes after starting a meal subcutaneously into the abdomen, upper arm, or thigh.
- Rotate injection sites within the same region from one injection to the next to reduce the risk of lipodystrophy and localized cutaneous amyloidosis. Do not inject into areas of lipodystrophy or localized cutaneous amyloidosis [see *Adverse Reactions (6.1, 6.2)*].
- FIASP given by subcutaneous injection should generally be used in regimens with intermediate or long-acting insulin.
- Instruct patients on basal-bolus treatment who forget a mealtime dose to monitor their blood glucose level to decide if an insulin dose is needed, and to resume their usual dosing schedule at the next meal.
- The FIASP FlexTouch pen dials in 1 unit increments.

Continuous Subcutaneous Infusion (Insulin Pump):

- Refer to the continuous subcutaneous insulin infusion pump user manual to see if FIASP or FIASP PumpCart can be used with the insulin pump. Use FIASP and FIASP PumpCart in accordance with the insulin pump system's instructions for use.
- Administer FIASP by continuous subcutaneous infusion in a region recommended in the instructions from the pump manufacturer. Rotate infusion sites within the same region to reduce the risk of lipodystrophy and localized cutaneous amyloidosis. Do not infuse into areas of lipodystrophy or localized cutaneous amyloidosis [see *Warnings and Precautions (5.2) Adverse Reactions (6.1)*].
- Train patients using continuous subcutaneous insulin infusion therapy to administer insulin by injection and have alternate insulin therapy available in case of insulin pump failure [see *Warnings and Precautions (5.8)*].
- Change FIASP in the pump reservoir at least every 6 days or replace the PumpCart cartridge at least every 4 days, or according to the pump user manual, whichever is shorter. Follow the FIASP-specific information for in-use time because FIASP-specific information may differ from general insulin pump user manual instructions.
- Change the infusion sets and the infusion set insertion site according to the manufacturers user manual.
- Do not mix with other insulins or diluents in the insulin pump.
- Do not expose FIASP in the pump reservoir to temperatures greater than 37°C (98.6°F).

Intravenous Administration:

- Administer FIASP intravenously **only** under medical supervision with close monitoring of blood glucose and potassium levels to avoid hypoglycemia and hypokalemia [see *Warnings and Precautions (5.3, 5.5)*].
- Dilute FIASP to concentrations from 0.5 unit/mL to 1 unit/mL insulin aspart in infusion systems using polypropylene infusion bags.

- FIASP is stable at room temperature at 20°C to 25°C (68°F to 77°F) for 24 hours in 0.9% sodium chloride or 5% dextrose infusion fluids.

2.3 Dosage Recommendations

- Individualize the dosage of FIASP based on the route of administration, patient's metabolic needs, blood glucose monitoring results, and glycemic control goal.
- If converting from another mealtime insulin to FIASP, the initial change can be done on a unit-to-unit basis.
- Dose adjustments may be needed when switching from another insulin, with changes in physical activity, changes in concomitant medications, changes in meal patterns (i.e., macronutrient content or timing of food intake), changes in renal or hepatic function or during acute illness to minimize the risk of hypoglycemia or hyperglycemia [see *Warnings and Precautions (5.2, 5.3) and Drug Interactions (7), and Use in Specific Populations (8.6, 8.7)*].
- Closely monitor blood glucose when converting insulins used in insulin pumps as individualization of insulin pump parameters may be necessary to minimize the risk of hypoglycemia and hyperglycemia [see *Warnings and Precautions (5.2, 5.3) and Adverse Reactions (6.1)*].
- During changes to a patient's insulin regimen, increase the frequency of blood glucose monitoring [see *Warnings and Precautions (5.2)*].
- Dosage adjustment may be needed when FIASP is co-administered with certain drugs [see *Drug Interactions (7)*].

3 DOSAGE FORMS AND STRENGTHS

Injection: 100 units of insulin aspart per mL (U-100) is available as a clear and colorless solution in:

- 10 mL multiple-dose vial
- 3 mL single-patient-use FIASP FlexTouch pen
- 3 mL single-patient-use PenFill cartridges for use in a PenFill cartridge delivery device
- 1.6 mL single-patient-use PumpCart cartridges for use in a compatible insulin pump.

4 CONTRAINDICATIONS

FIASP is contraindicated:

- During episodes of hypoglycemia [see *Warnings and Precautions (5.3)*].
- In patients with known hypersensitivity to insulin aspart or any of the excipients in FIASP [see *Warnings and Precautions (5.6)*].

5 WARNINGS AND PRECAUTIONS

5.1 Never Share a FIASP FlexTouch Pen, PenFill Cartridge or PenFill Cartridge Device Between Patients

FIASP FlexTouch disposable pen, PenFill cartridge and PenFill cartridge devices should

never be shared between patients, even if the needle is changed. Patients using FIASP vials should never share needles or syringes with another person. Sharing poses a risk for transmission of blood-borne pathogens.

5.2 Hyperglycemia or Hypoglycemia with Changes in Insulin Regimen

Changes in an insulin regimen (e.g., insulin strength, manufacturer, type, injection site or method of administration) may affect glycemic control and predispose to hypoglycemia [see *Warnings and Precautions (5.3)*] or hyperglycemia. Repeated insulin injections into areas of lipodystrophy or localized cutaneous amyloidosis have been reported to result in hyperglycemia; and a sudden change in the injection site (to an unaffected area) has been reported to result in hypoglycemia [see *Adverse Reactions (6.1, 6.2)*].

Make any changes to a patient's insulin regimen under close medical supervision with increased frequency of blood glucose monitoring. Advise patients who have repeatedly injected into areas of lipodystrophy or localized cutaneous amyloidosis to change the injection site to unaffected areas and closely monitor for hypoglycemia. For patients with type 2 diabetes mellitus, dosage adjustments in concomitant anti-diabetic treatment may be needed.

5.3 Hypoglycemia

Hypoglycemia is the most common adverse reaction of all insulin therapies, including FIASP [see *Adverse Reactions (6.1)*]. Severe hypoglycemia can cause seizures, may lead to unconsciousness, may be life-threatening, or cause death. Hypoglycemia can impair concentration ability and reaction time; this may place an individual and others at risk in situations where these abilities are important (e.g., driving or operating other machinery). FIASP, or any insulin, should not be used during episodes of hypoglycemia [see *Contraindications (4)*].

Hypoglycemia can happen suddenly and symptoms may differ in each individual and change over time in the same individual. Symptomatic awareness of hypoglycemia may be less pronounced in patients with longstanding diabetes, in patients with diabetic nerve disease, in patients using medications that block the sympathetic nervous system (e.g., beta-blockers) [see *Drug Interactions (7)*], or in patients who experience recurrent hypoglycemia.

Risk Factors for Hypoglycemia

The risk of hypoglycemia after an injection is related to the duration of action of the insulin and, in general, is highest when the glucose lowering effect of the insulin is maximal. The timing of hypoglycemia usually reflects the time-action profile of the administered insulin formulation. As with all insulin preparations, the glucose lowering effect time course of FIASP may vary in different individuals or at different times in the same individual and depends on many conditions, including the area of injection as well as the injection site blood supply and temperature [see *Use in Specific Populations (8.4), Clinical Pharmacology (12.2)*].

Other factors which may increase the risk of hypoglycemia include changes in meal pattern (e.g., macronutrient content or timing of meals), changes in level of physical activity, or changes to co-administered medication [see *Drug Interactions (7)*]. Patients with renal or hepatic impairment may be at higher risk of hypoglycemia [see *Use in Specific Populations (8.6, 8.7)*].

Risk Mitigation Strategies for Hypoglycemia

Patients and caregivers must be educated to recognize and manage hypoglycemia. Self-monitoring of blood glucose plays an essential role in the prevention and management of hypoglycemia. In patients at higher risk for hypoglycemia and patients who have reduced symptomatic awareness of hypoglycemia, increased frequency of blood glucose monitoring is recommended.

5.4 Hypoglycemia Due to Medication Errors

Accidental mix-ups between insulin products have been reported. To avoid medication errors between FIASP and other insulins, instruct patients to always check the insulin label before each injection.

5.5 Hypokalemia

All insulin products, including FIASP, can cause a shift in potassium from the extracellular to intracellular space, possibly leading to hypokalemia. Untreated hypokalemia may cause respiratory paralysis, ventricular arrhythmia and death. Monitor potassium levels in patients at risk for hypokalemia if indicated (e.g., patients using potassium-lowering medications, patients taking medications sensitive to potassium concentrations).

5.6 Hypersensitivity and Allergic Reactions

Severe, life-threatening, generalized allergy, including anaphylaxis, can occur with insulin products, including FIASP [see *Adverse Reactions (6.1)*]. If hypersensitivity reactions occur, discontinue FIASP; treat per standard of care and monitor until symptoms and signs resolve. FIASP is contraindicated in patients who have had hypersensitivity reactions to insulin aspart, or any of the excipients in FIASP [see *Contraindications (4)*].

5.7 Fluid Retention and Heart Failure with Concomitant Use of PPAR-Gamma Agonists

Thiazolidinediones (TZDs), which are peroxisome proliferator-activated receptor (PPAR)-gamma agonists, can cause dose-related fluid retention, particularly when used in combination with insulin. Fluid retention may lead to or exacerbate heart failure. Patients treated with insulin, including FIASP, and a PPAR-gamma agonist should be observed for signs and symptoms of heart failure. If heart failure develops, it should be managed according to current standards of care, and discontinuation or dose reduction of the PPAR-gamma agonist must be considered.

5.8 Hyperglycemia and Ketoacidosis Due to Insulin Pump Device Malfunction

Pump or infusion set malfunctions can lead to a rapid onset of hyperglycemia and ketoacidosis. Prompt identification and correction of the cause of hyperglycemia or ketosis is necessary. Interim therapy with subcutaneous injection of FIASP may be required. Patients using continuous subcutaneous insulin infusion pump therapy must be trained to administer insulin by injection and have alternate insulin therapy available in case of pump failure [see *Dosage and Administration (2.2)*, *How Supplied/Storage and Handling (16.2)*, and *Patient Counseling Information (17)*].

6 ADVERSE REACTIONS

The following clinically significant adverse reactions are described elsewhere in labeling:

- Hyperglycemia or Hypoglycemia with Changes in Insulin Regimen [see Warnings and Precautions (5.2)]
- Hypoglycemia [see Warnings and Precautions (5.3)]
- Hypokalemia [see Warnings and Precautions (5.5)]
- Hypersensitivity and allergic reactions [see Warnings and Precautions (5.6)]

6.1 Clinical Trial Experience

Because clinical trials are conducted under widely varying conditions, adverse reaction rates observed in the clinical trials of a drug cannot be directly compared to rates in the clinical trials of another drug, and may not reflect the rates actually observed in clinical practice.

The data in Table 1 reflect the exposure of 763 adult patients with type 1 diabetes mellitus to FIASP in one clinical trial with a mean exposure duration of 25 weeks [see Clinical Studies (14.2)]. The mean age was 44.4 years and the mean duration of diabetes was 19.9 years. 59% were male, 93% were White, and 2% were Black or African American; and 7% were Hispanic or Latino. The mean BMI was 26.7 kg/m² and the mean HbA_{1c} at baseline was 7.6%.

The data in Table 2 reflect the exposure of 341 adult patients with type 2 diabetes mellitus to FIASP in one clinical trial with a mean exposure duration of 24 weeks [see Clinical Studies (14)]. The mean age was 59.6 years and the mean duration of diabetes was 13.2 years. 47% were male, 80% were White, and 6% were Black or African American; and 8% were Hispanic or Latino. The mean BMI was 31.5 kg/m² and the mean HbA_{1c} at baseline was 8.0%.

The data in Table 3 reflect the exposure of 519 pediatric patients with type 1 diabetes mellitus to FIASP in one clinical trial with a mean exposure duration of 26 weeks [see Clinical Studies (14.3)]. The mean age was 11.7 years and the mean duration of diabetes mellitus was 4.4 years. 54% were male, 81% were White, 16% were Asian and 2% were Black or African American. The mean BMI was 19.7 kg/m² and the mean HbA_{1c} at baseline was 7.6%.

Common adverse reactions, excluding hypoglycemia, were defined as events occurring in ≥5% and occurring at the same rate or greater for FIASP-treated patients than comparator-treated patients.

Table 1. Adverse Reactions (%*) in Adult Patients with Type 1 Diabetes Mellitus

	Mealtime FIASP + Insulin detemir (N=386)	Postmeal FIASP + Insulin detemir (N=377)
Nasopharyngitis	20.2	23.9
Upper respiratory tract infection	9.1	7.4
Nausea	4.9	5.0
Diarrhea	5.4	3.2

Back pain	5.2	4.0
-----------	-----	-----

*Incidence \geq 5% and occurring at the same rate or greater with FIASP than comparator

Table 2. Adverse Reactions (%*) in Adult Patients with Type 2 Diabetes Mellitus

	FIASP + Insulin glargine (N=341)
Urinary tract infection	5.9

*Incidence \geq 5% and occurring at the same rate or greater with FIASP than comparator

Table 3: Adverse Reactions (%*) in Pediatric Patients with Type 1 Diabetes Mellitus

	Mealtime FIASP + Insulin degludec (N=261)	Postmeal FIASP + Insulin degludec (N=258)
Viral upper respiratory tract infection	23.0	20.5
Upper respiratory tract infection	8.4	12.4
Influenza	7.7	5.8
Rhinitis	3.8	6.2
Headache	6.1	10.1
Pyrexia	8.4	6.2
Vomiting	3.4	8.1

*Incidence \geq 5% and occurring at the same rate or greater with FIASP than comparator

Hypoglycemia

Hypoglycemia is the most commonly observed adverse reaction in patients using insulin, including FIASP. The rates of reported hypoglycemia depend on the definition of hypoglycemia used, diabetes type, insulin dose, intensity of glucose control, background therapies, and other intrinsic and extrinsic patient factors. For these reasons, comparing rates of hypoglycemia in clinical trials for FIASP with the incidence of hypoglycemia for other products may be misleading and also, may not be representative of hypoglycemia rates that occur in clinical practice.

Incidence rates for severe hypoglycemia in adults with type 1 and type 2 diabetes mellitus and pediatric patients with type 1 diabetes mellitus treated with FIASP in clinical trials are shown in Table 4 [see *Clinical Studies (14)*].

Table 4. Proportion (%) of Patients with Type 1 Diabetes and Type 2 Diabetes Mellitus Experiencing at Least One Episode of Severe Hypoglycemia in Adult and Pediatric Clinical Trials

	Study A (Type 1) Adults	Study B (Type 2)	Study E (Type 1) Pediatric	Study D (Type 1 CSII)
--	------------------------------------	-----------------------------	---------------------------------------	----------------------------------

			Adults			
	Mealtime FIASP + Insulin detemir (N=386)	Postmeal FIASP + Insulin detemir (N=377)	FIASP + Insulin glargine (N=341)	Mealtime FIASP + Insulin degludec (N=261)	Postmeal FIASP + Insulin degludec (N=258)	FIASP (N=236)
Severe hypoglycemia*	6.7	8.0	3.2	1.1	3.1	4.7

*Severe hypoglycemia: an episode requiring assistance of another person to actively administer carbohydrate, glucagon, or other resuscitative actions

Blood glucose confirmed hypoglycemia was defined as a self-measured glucose calibrated to plasma of less than 56 mg/dL.

In Study D, adult patients with type 1 diabetes mellitus treated with FIASP in a pump reported a higher rate of blood glucose confirmed hypoglycemic episodes within the first hour after a meal compared to patients treated with NovoLog [see *Clinical Trials (14.5)*].

In Study E, pediatric patients with type 1 diabetes mellitus treated with mealtime and postmeal FIASP reported a higher rate of blood glucose confirmed hypoglycemic episodes compared to patients treated with NovoLog; the imbalance was greater during the nocturnal period [see *Use in Specific Populations (8.4), Clinical Trials (14.3)*].

Allergic Reactions

Severe, life-threatening, generalized allergy, including anaphylaxis, generalized skin reactions, angioedema, bronchospasm, hypotension, and shock may occur with any insulin, including FIASP, and may be life threatening. In the clinical program, generalized hypersensitivity reactions (manifested by generalized skin rash and facial edema) were reported in 0.4% of adult patients treated with FIASP. Allergic skin manifestations reported with FIASP in 1.7% of adult patients from the clinical program include eczema, rash, rash pruritic, urticaria and dermatitis. In Study D, allergic reactions were reported in 4.2% of adult patients with type 1 diabetes mellitus treated with FIASP. In Study E, allergic reactions were reported in 4% of pediatric patients with type 1 diabetes mellitus treated with FIASP.

Lipodystrophy

Administration of insulin, including FIASP, has resulted in lipohypertrophy (enlargement or thickening of tissue) and lipoatrophy (depression in the skin). In the clinical program, lipodystrophy was reported in 0.4% of adult patients and 2.1% of pediatric patients treated with FIASP [see *Dosage and Administration (2.2)*].

Injection/Infusion Site Reactions

As with other insulin therapy, patients may experience rash, redness, inflammation, pain, bruising or itching at the site of FIASP injection or infusion. These reactions usually resolve in a few days to a few weeks, but in some occasions, may require discontinuation of FIASP. In the clinical program, injection site reactions occurred in 1.6% of adult patients treated with FIASP. In Study A, adult patients with type 1 diabetes mellitus treated with FIASP reported 2.2% injection site reactions. In Study D, infusion site reactions were reported in 10.2% of adult patients with type 1 diabetes mellitus

treated with FIASP. In Study E, injection site reactions were reported in 4.2% of pediatric patients with type 1 diabetes mellitus treated with FIASP.

Weight Gain

Weight gain can occur with insulin therapy, including FIASP, and has been attributed to the anabolic effects of insulin and the decrease in glucosuria. In Study A, adult patients with type 1 diabetes mellitus treated with FIASP gained an average of 0.7 kg and in Study B, adult patients with type 2 diabetes mellitus treated with FIASP gained an average of 2.7 kg.

Peripheral Edema

Insulin, including FIASP, may cause sodium retention and edema, particularly if previous poor metabolic control is improved by intensified insulin therapy. In the clinical program, peripheral edema occurred in 0.8% of adult patients treated with FIASP.

6.2 Postmarketing Experience

The following additional adverse reactions have been identified during post-approval use of insulin aspart. Because these reactions are reported voluntarily from a population of uncertain size, it is not always possible to reliably estimate their frequency or establish a causal relationship to drug exposure.

Localized cutaneous amyloidosis at the injection site has occurred. Hyperglycemia has been reported with repeated insulin injections into areas of localized cutaneous amyloidosis; hypoglycemia has been reported with a sudden change to an unaffected injection site.

7 DRUG INTERACTIONS

Table 5 includes clinically significant drug interactions with FIASP.

Table 5. Clinically Significant Drug Interactions with FIASP

Drugs That May Increase the Risk of Hypoglycemia	
<i>Drugs:</i>	Antidiabetic agents, ACE inhibitors, angiotensin II receptor blocking agents, disopyramide, fibrates, fluoxetine, monoamine oxidase inhibitors, pentoxifylline, pramlintide, salicylates, somatostatin analogs (e.g., octreotide), and sulfonamide antibiotics.
<i>Intervention:</i>	Dose reductions and increased frequency of glucose monitoring may be required when FIASP is co-administered with these drugs.
Drugs That May Decrease the Blood Glucose Lowering Effect of FIASP	
<i>Drugs:</i>	Atypical antipsychotics (e.g., olanzapine and clozapine), corticosteroids, danazol, diuretics, estrogens, glucagon, isoniazid, niacin, oral contraceptives, phenothiazines, progestogens (e.g., in oral contraceptives), protease inhibitors, somatropin, sympathomimetic agents (e.g., albuterol, epinephrine, terbutaline), and thyroid hormones.
<i>Intervention:</i>	Dose increases and increased frequency of glucose monitoring may be required when FIASP is co-administered with these drugs.
Drugs That May Increase or Decrease the Blood Glucose Lowering Effect of	

FIASP	
<i>Drugs:</i>	Alcohol, beta-blockers, clonidine, and lithium salts. Pentamidine may cause hypoglycemia, which may sometimes be followed by hyperglycemia.
<i>Intervention:</i>	Dose adjustment and increased frequency of glucose monitoring may be required when FIASP is co-administered with these drugs.
Drugs That May Blunt Signs and Symptoms of Hypoglycemia	
<i>Drugs:</i>	Beta-blockers, clonidine, guanethidine, and reserpine.
<i>Intervention:</i>	Increased frequency of glucose monitoring may be required when FIASP is co-administered with these drugs.

8 USE IN SPECIFIC POPULATIONS

8.1 Pregnancy

Risk Summary

There are no available data with FIASP in pregnant women to inform a drug-associated risk for major birth defects and miscarriage. Available information from published randomized controlled trials with insulin aspart use during the second trimester of pregnancy have not reported an association with insulin aspart and major birth defects or adverse maternal or fetal outcomes [see Data]. There are risks to the mother and fetus associated with poorly controlled diabetes in pregnancy [see Clinical Considerations].

In animal reproduction studies, administration of subcutaneous insulin aspart to pregnant rats and rabbits during the period of organogenesis did not cause adverse developmental effects at exposures 8- times and equal to the human subcutaneous dose of 1.0 unit/kg/day, respectively. Pre- and post-implantation losses and visceral/skeletal abnormalities were seen at higher exposures, which are considered secondary to maternal hypoglycemia. These effects were similar to those observed in rats administered regular human insulin [see Data].

The estimated background risk of major birth defects is 6-10% in women with pre-gestational diabetes with a HbA_{1c} >7% and has been reported to be as high as 20-25% in women with a HbA_{1c} >10%. The estimated background risk of miscarriage for the indicated population is unknown. In the U.S. general population, the estimated background risk of major birth defects and miscarriage in clinically recognized pregnancies is 2-4% and 15-20%, respectively.

Clinical Considerations

Disease-Associated Maternal and/or Embryo-Fetal Risk

Poorly controlled diabetes in pregnancy increases the maternal risk for diabetic ketoacidosis, preeclampsia, spontaneous abortions, preterm delivery, and delivery complications. Poorly controlled diabetes increases the fetal risk for major birth defects, stillbirth, and macrosomia related morbidity.

Data

Human Data

Published data from 5 randomized controlled trials of 441 pregnant women with diabetes mellitus treated with insulin aspart starting during the late 2nd trimester of pregnancy did not identify an association of insulin aspart with major birth defects or adverse maternal or fetal outcomes. However, these studies cannot definitely establish the absence of any risk because of methodological limitations, including a variable duration of treatment and small size of the majority of the trials.

Animal Data

Fertility, embryo-fetal and pre- and postnatal development studies have been performed with insulin aspart and regular human insulin in rats and rabbits. In a combined fertility and embryo-fetal development study in rats, insulin aspart was administered before mating, during mating, and throughout pregnancy. Further, in a pre- and postnatal development study insulin aspart was given throughout pregnancy and during lactation to rats. In an embryo-fetal development study insulin aspart was given to female rabbits during organogenesis. The effects of insulin aspart did not differ from those observed with subcutaneous regular human insulin. Insulin aspart, like human insulin, caused pre- and post-implantation losses and visceral/skeletal abnormalities in rats at a dose of 200 units/kg/day (approximately 32 times the human subcutaneous dose of 1.0 unit/kg/day, based on human exposure equivalents) and in rabbits at a dose of 10 units/kg/day (approximately three times the human subcutaneous dose of 1.0 unit/kg/day, based on human exposure equivalents). No significant effects were observed in rats at a dose of 50 units/kg/day and in rabbits at a dose of 3 units/kg/day. These doses are approximately 8 times the human subcutaneous dose of 1.0 unit/kg/day for rats and equal to the human subcutaneous dose of 1.0 unit/kg/day for rabbits, based on human exposure equivalents. The effects are considered secondary to maternal hypoglycemia.

8.2 Lactation

Risk Summary

There are no data on the presence of FIASP in human milk, the effects on the breastfed infant, or the effect on milk production. One small published study reported that exogenous insulin, including insulin aspart, was present in human milk. However, there is insufficient information to determine the effects of insulin aspart on the breastfed infant and no available information on the effects of insulin aspart on milk production. The developmental and health benefits of breastfeeding should be considered along with the mother's clinical need for insulin, any potential adverse effects on the breastfed child from FIASP or insulin aspart or from the underlying maternal condition.

8.4 Pediatric Use

The safety and effectiveness of FIASP have been established to improve glycemic control in pediatric patients with diabetes mellitus. Use of FIASP for this indication is supported by evidence from an adequate and well-controlled study in 777 pediatric patients with type 1 diabetes mellitus aged 2 to 17 years, and from studies in adults with diabetes mellitus [see *Clinical Pharmacology (12.3)* and *Clinical Studies (14)*].

Pediatric patients with type 1 diabetes mellitus treated with mealtime and postmeal FIASP reported a higher rate of blood glucose confirmed hypoglycemic episodes compared to patients treated with NovoLog; the imbalance was greater during the nocturnal period. Monitor blood glucose levels closely in pediatric patients [see *Warnings and Precautions (5.3)*, *Clinical Trial Experience (6.1)*].

8.5 Geriatric Use

In the three controlled clinical studies, 192 of 1219 (16%) FIASP treated patients with type 1 or type 2 diabetes mellitus were \geq 65 years of age and 24 of 1219 (2%) were \geq 75 years of age. No overall differences in safety or effectiveness were observed between these elderly patients and younger adult patients.

Nevertheless, caution should be exercised when FIASP is administered to geriatric patients. In elderly patients with diabetes, the initial dosing, dose increments, and maintenance dosage should be conservative to avoid hypoglycemia [see *Warnings and Precautions (5.3)*, *Adverse Reactions (6.1)* and *Clinical Studies (14)*].

Pharmacokinetic/pharmacodynamic study to assess the effect of age on the onset of FIASP action has been performed [see *Clinical Pharmacology (12.3)*].

8.6 Renal Impairment

Patients with renal impairment may be at increased risk of hypoglycemia and may require more frequent FIASP dose adjustment and more frequent blood glucose monitoring [see *Warnings and Precautions (5.3)* and *Clinical Pharmacology (12.3)*].

8.7 Hepatic Impairment

Patients with hepatic impairment may be at increased risk of hypoglycemia and may require more frequent FIASP dose adjustment and more frequent blood glucose monitoring [see *Warnings and Precautions (5.3)* and *Clinical Pharmacology (12.3)*].

10 OVERDOSAGE

Excess insulin administration may cause hypoglycemia and hypokalemia [see *Warnings and Precautions (5.3, 5.5)*]. Mild episodes of hypoglycemia usually can be treated with oral glucose. Adjustments in drug dosage, meal patterns, or exercise, may be needed. More severe episodes with coma, seizure or neurologic impairment may be treated with an intramuscular/subcutaneous glucagon product for emergency use or concentrated intravenous glucose. Sustained carbohydrate intake and observation may be necessary because hypoglycemia may recur after apparent clinical recovery. Hypokalemia must be corrected appropriately.

11 DESCRIPTION

Insulin aspart is a rapid-acting insulin analog for subcutaneous or intravenous administration. Insulin aspart is homologous with regular human insulin with the exception of a single substitution of the amino acid proline by aspartic acid in position B28, and is produced by recombinant DNA technology utilizing *Saccharomyces cerevisiae*. Insulin aspart has the empirical formula $C_{256}H_{381}N_{65}O_{79}S_6$ and a molecular weight of 5825.8 daltons.

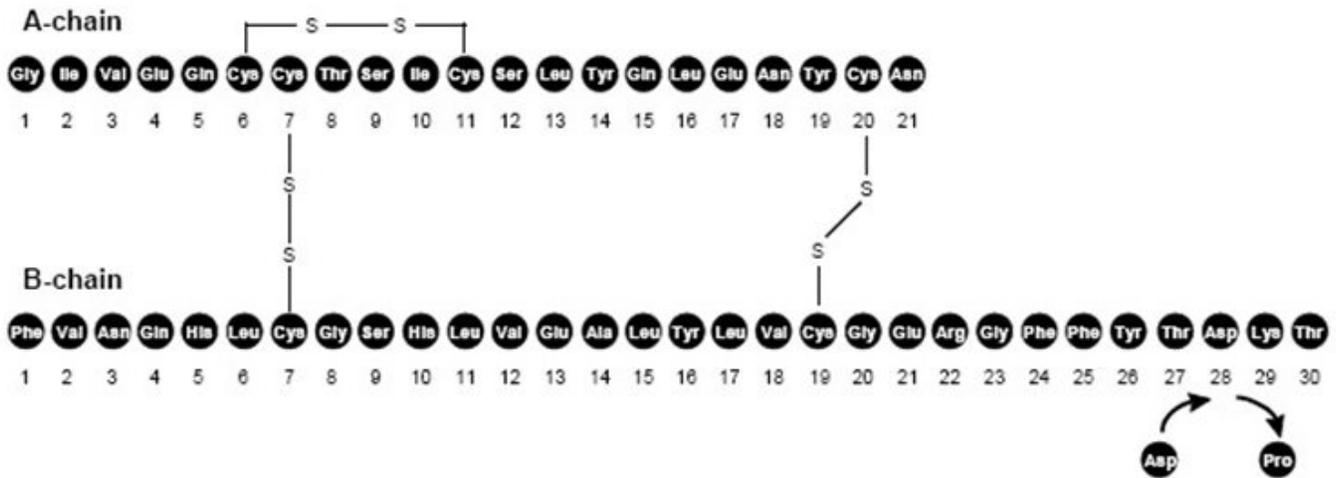


Figure 1. Structural formula of insulin aspart

FIASP (insulin aspart) injection is an aqueous, sterile, clear and colorless solution. Each mL contains 100 units of insulin aspart and the inactive ingredients: arginine (as L-arginine hydrochloride), USP (3.48 mg); dibasic sodium phosphate, USP (0.42 mg); glycerin, USP (3.3 mg); metacresol, USP (1.72 mg); niacinamide, USP (20.8 mg); phenol, USP (1.50 mg); zinc (as zinc acetate), USP (19.6 mcg) and Water for Injection. Hydrochloric acid and/or sodium hydroxide may be added to adjust pH to 7.1.

12 CLINICAL PHARMACOLOGY

12.1 Mechanism of Action

The primary activity of FIASP is the regulation of glucose metabolism. Insulins, including insulin aspart, the active ingredient in FIASP, exert their specific action through binding to insulin receptors. Receptor-bound insulin lowers blood glucose by facilitating cellular uptake of glucose into skeletal muscle and adipose tissue and by inhibiting the output of glucose from the liver. Insulin inhibits lipolysis in the adipocyte, inhibits proteolysis, and enhances protein synthesis.

12.2 Pharmacodynamics

The time course of insulin action (i.e., glucose lowering) may vary considerably in different individuals or within the same individual. The average pharmacodynamic profile (i.e., glucose lowering effect measured as glucose infusion rate (GIR) in a euglycemic clamp study) for subcutaneous administration of 0.1, 0.2, and 0.4 unit/kg of FIASP in 46 patients with Type 1 diabetes mellitus is shown in Figure 2 and key characteristics of the timing of the effect are described in Table 6 below.

Table 6. Timing of insulin effect (i.e., mean pharmacodynamic effect) after subcutaneous administration of 0.1, 0.2 and 0.4 unit/kg of FIASP in patients (N=46) with Type 1 Diabetes Mellitus and corresponding to the data shown in Figure 2

Parameter for Insulin Effect	FIASP 0.1 unit/kg	FIASP 0.2 unit/kg	FIASP 0.4 unit/kg
------------------------------	-------------------	-------------------	-------------------

Time to first measurable effect	~20 minutes	~17 minutes	~16 minutes
Time to peak effect	~91 minutes	~122 minutes	~133 minutes
Time for effect to return to baseline	~5 hours	~6 hours	~7 hours

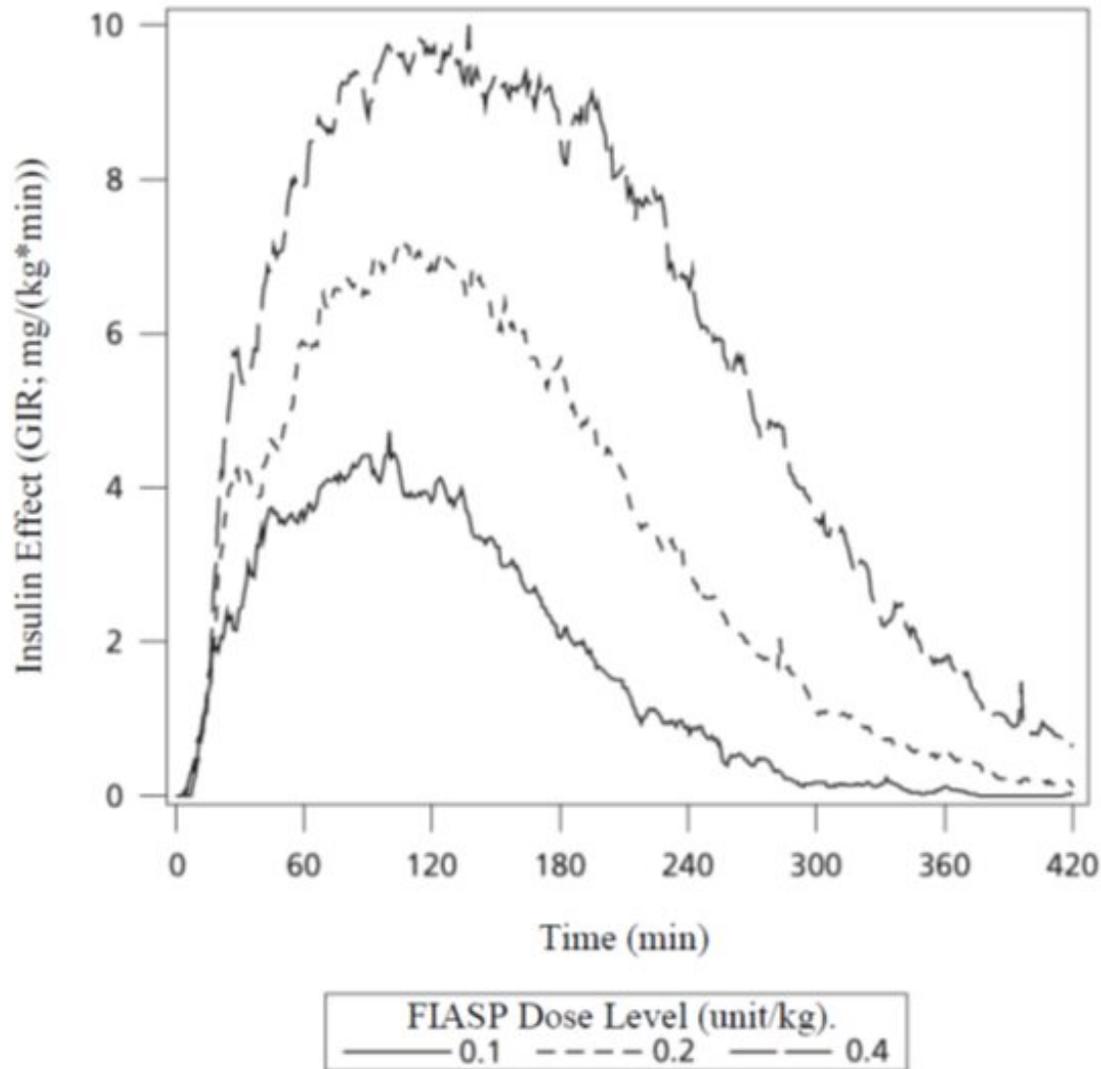


Figure 2. Mean insulin effect (i.e., mean pharmacodynamic effect) over time after subcutaneous administration of 0.1, 0.2 and 0.4 unit/kg of FIASP in patients (N=46) with Type 1 Diabetes Mellitus

On average, the pharmacodynamic effects of FIASP, measured as area under the glucose infusion rate-time curve (AUC_{GIR}), was 697 mg/kg, 1406 mg/kg, and 2427 mg/kg following administration of 0.1, 0.2, and 0.4 unit/kg of FIASP.

The day-to-day variability in glucose-lowering-effect of FIASP within patients was ~18% for total glucose lowering ($AUC_{GIR, 0-12h}$) and ~19% for maximum glucose lowering effect (GIR_{max}).

12.3 Pharmacokinetics

Absorption

Pharmacokinetic results from a euglycemic clamp study in adult patients with type 1 diabetes mellitus (N=51) showed that insulin aspart appeared in the circulation ~2.5 minutes after administration of FIASP (Figure 3). Time to maximum insulin concentrations was achieved ~63 minutes after administration of FIASP.

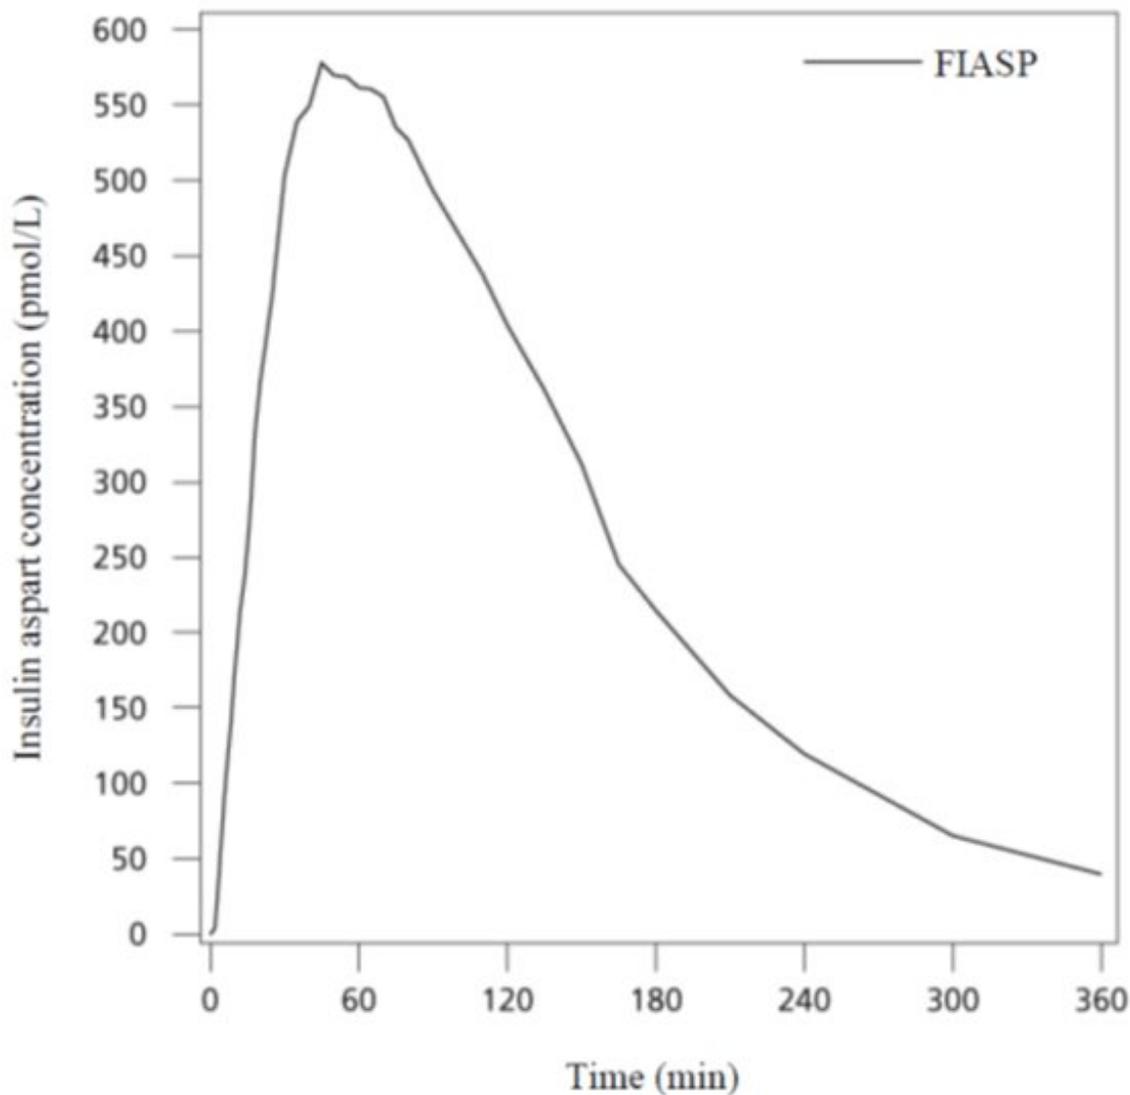


Figure 3. Mean Insulin Aspart Serum Concentration Profile in Adult Subjects with Type 1 Diabetes Mellitus (N=51) following a single 0.2 unit/kg dose (subcutaneous) of FIASP

Total insulin exposure and maximum insulin concentration increase proportionally with increasing subcutaneous dose of FIASP within the therapeutic dose range.

Distribution

Insulin aspart has a low binding affinity to plasma proteins (<10%), similar to that seen with regular human insulin.

Elimination

The apparent terminal half-life after subcutaneous administration of FIASP is about 1.1 hours.

Specific Populations

Age, gender, BMI, and race did not meaningfully affect the pharmacokinetics and pharmacodynamics of FIASP.

Patients with Renal and Hepatic Impairment

Based on studies conducted with insulin aspart, renal and hepatic impairment is not known to impact the pharmacokinetics of insulin aspart.

12.6 Immunogenicity

The observed incidence of anti-drug antibodies is highly dependent on the sensitivity and specificity of the assay. Differences in assay methods preclude meaningful comparisons of the incidence of anti-drug antibodies in the studies described below with the incidence of anti-drug antibodies in other studies, including those of FIASP or of other insulin aspart products.

In a 26-week study in adult subjects with type 1 diabetes mellitus (Study A) [see *Clinical Studies (14.2)*], among the 763 subjects who received FIASP, 97% were positive for cross-reacting anti-insulin antibodies (AIA) at least once during the study, including 90% that were positive at baseline. A total of 25% of patients who received FIASP were positive for anti-drug (insulin aspart) antibodies (ADA) at least once during the study, including 17% that were positive at baseline.

In a 26-week study in pediatric subjects with type 1 diabetes mellitus (Study E) [see *Clinical Studies (14.3)*], among the 519 subjects who received FIASP, 97% were positive for cross-reacting AIA at least once during the study, including 95% that were positive at baseline. A total of 19% of patients who received FIASP were positive for ADA at least once during the study, including 16.0% that were positive at baseline.

There was no identified clinically significant effect of ADA on pharmacokinetics, pharmacodynamics, safety, or effectiveness of FIASP.

13 NONCLINICAL TOXICOLOGY

13.1 Carcinogenesis, Mutagenesis, Impairment of Fertility

In 52-week studies, Sprague-Dawley rats were dosed subcutaneously with insulin aspart at 10, 50, and 200 units/kg/day (approximately 2, 8, and 32 times the human subcutaneous dose of 1.0 units/kg/day, based on units/body surface area, respectively). At a dose of 200 units/kg/day, insulin aspart increased the incidence of mammary gland tumors in females when compared to untreated controls. The incidence of mammary tumors for insulin aspart was not significantly different than for regular human insulin. The relevance of these findings to humans is not known.

Insulin aspart was not genotoxic in the following tests: Ames test, mouse lymphoma cell forward gene mutation test, human peripheral blood lymphocyte chromosome aberration test, *in vivo* micronucleus test in mice, and *in vivo* UDS test in rat liver hepatocytes.

In fertility studies in male and female rats, at subcutaneous doses up to 200 units/kg/day (approximately 32 times the human subcutaneous dose, based on units/body surface area), no direct adverse effects on male and female fertility, or general reproductive performance of animals was observed.

14 CLINICAL STUDIES

14.1 Overview of Clinical Studies

The efficacy of FIASP was evaluated in 3 randomized, active-controlled trials of 18 to 26 weeks duration in adults and one randomized, active-controlled, treat-to-target trial of 26 weeks duration in pediatric patients.

In total 1,224 adult subjects (N=763 with type 1 diabetes mellitus; N=461 with type 2 diabetes mellitus) and 519 pediatric subjects with type 1 diabetes mellitus were randomized to FIASP. In adult and pediatric patients with type 1 diabetes mellitus, mealtime FIASP and postmeal FIASP led to non-inferior glycemic control compared to mealtime NovoLog, both in combination with basal insulin. In adult patients with type 2 diabetes mellitus, mealtime FIASP provided non-inferior glycemic control compared to mealtime NovoLog, both in combination with metformin. In addition, mealtime FIASP in a basal-bolus regimen with metformin also provided statistically significant improvement in the overall glycemic control compared to basal insulin therapy alone with metformin in adult patients with type 2 diabetes mellitus.

In adults with type 1 diabetes mellitus (N=472), FIASP led to non-inferior glycemic control compared to NovoLog when both were administered by continuous subcutaneous insulin infusion (CSII) pump.

14.2 Type 1 Diabetes Mellitus - Adults

Study A (NCT01831765): FIASP added to insulin detemir in adult patients with Type 1 Diabetes Mellitus inadequately controlled at baseline.

The efficacy of FIASP was evaluated in a 26-week, randomized, active controlled, treat-to-target, multicenter trial in 1,143 adult patients with type 1 diabetes mellitus inadequately controlled at baseline. Patients were randomized to either blinded mealtime FIASP (N=381), blinded mealtime NovoLog (N=380), or open-label postmeal FIASP (N=382), all in combination with once or twice daily insulin detemir. At randomization, patients were switched to FIASP on a unit to unit basis. Mealtime FIASP or NovoLog was injected 0-2 minutes before the meal, and postmeal FIASP was injected 20 minutes after the start of the meal.

The mean age of the randomized subjects was 44.4 years and mean duration of diabetes was 19.9 years. 59% were male, 93% were White and 2% were Black or African American; and 7% were Hispanic or Latino. The mean BMI was 26.7 kg/m².

After 26 weeks of treatment, treatment difference in HbA_{1c} reduction from baseline between mealtime FIASP compared to mealtime NovoLog, and the treatment difference between postmeal FIASP compared to mealtime NovoLog met the pre-specified non-inferiority margin (0.4%). See Table 7. Insulin doses were similar among study arms at baseline and at the end of the trial.

Table 7. Results from Study A: 26-Week Trial of Mealtime FIASP and

Postmeal FIASP compared to Mealtime NovoLog Used in Combination with Insulin Detemir in Adults with Type 1 Diabetes Mellitus

	Mealtime FIASP + insulin detemir	Postmeal FIASP + insulin detemir	Mealtime NovoLog + insulin detemir
Number of subjects randomized (N)	381	382	380
HbA_{1c} (%)			
Baseline (mean)	7.6	7.6	7.6
Adjusted mean change from baseline	-0.32	-0.13	-0.17
Estimated treatment difference vs. mealtime NovoLog [95% CI]*	-0.15 [-0.23;-0.07]	0.04 [-0.04;0.12]	

Baseline is based on the mean of the observed last available values prior to randomization.

*Tested for non-inferiority

Estimated treatment difference was calculated using mixed model for repeated measurements (MMRM).

7.6% of subjects on the Mealtime FIASP arm, 7.6% of subjects on the Postmeal FIASP arm, and 5.3% of subjects on the Mealtime NovoLog arm were missing the final HbA_{1c} assessment.

14.3 Type 1 Diabetes Mellitus - Pediatric Patients

Study E (NCT02670915): FIASP added to insulin degludec in pediatric patients with Type 1 Diabetes Mellitus.

The efficacy of FIASP was evaluated in a 26-week, randomised, multinational, active controlled, treat-to-target, 3-armed parallel-group trial in 777 pediatric patients with type 1 diabetes mellitus. Patients were randomized to either blinded mealtime FIASP (N=260), blinded mealtime NovoLog (N=258), or open-label postmeal FIASP (N=259), all in combination with once daily insulin degludec. Mealtime FIASP or NovoLog was injected 0-2 minutes before the meal, and postmeal FIASP was injected 20 minutes after the start of the meal.

The mean age of the subjects at baseline was 11.7 years (range 2 to 17 years) and the mean duration of diabetes was 4.4 years. 54% were male, 81% were White, 16% were Asian and 2% were Black or African American. The mean BMI was 19.7 kg/m².

After 26 weeks of treatment, the treatment difference for change in HbA_{1c} from

baseline between mealtime FIASP compared to mealtime NovoLog, and the treatment difference between postmeal FIASP compared to mealtime NovoLog met the pre-specified non-inferiority margin (0.4%). See Table 8. Insulin doses were similar among study arms at baseline and at the end of the trial.

Table 8. Results from Study E: 26-Week Trial of Mealtime FIASP and Postmeal FIASP compared to Mealtime NovoLog Used in Combination with Insulin Degludec in Pediatrics with Type 1 Diabetes Mellitus

	Mealtime FIASP + insulin degludec	Postmeal FIASP + insulin degludec	Mealtime NovoLog + insulin degludec
Number of subjects randomized (N)	260	259	258
HbA_{1c} (%)			
Baseline (mean)	7.57	7.58	7.53
Adjusted mean change from baseline	0.06	0.35	0.22
Estimated treatment difference vs. mealtime NovoLog [95% CI]*	-0.17 [-0.30; -0.03]	0.13 [-0.01; 0.26]	

Baseline is based on the mean of the observed last available values prior to randomization.

*Tested for non-inferiority

Estimated treatment difference was calculated using ANCOVA. Week 26, change in HbA_{1c} was missing for 1.5%, 1.9%, and 1.6% of subjects in mealtime FIASP, post-meal FIASP, and NovoLog respectively. Missing values were imputed with a missing at random assumption.

14.4 Type 2 Diabetes Mellitus - Adults

Study B (NCT01819129): FIASP added to basal insulin and oral antidiabetics in patients with Type 2 Diabetes Mellitus inadequately controlled at baseline on basal insulin and oral antidiabetics

The efficacy of FIASP was evaluated in a 26-week randomized, double-blind, active controlled, treat-to-target, multicenter, multinational, parallel group trial in 689 adult patients with type 2 diabetes mellitus who were inadequately controlled at baseline on basal insulin and oral antidiabetic therapy and had been on these therapies for at least 6 months. Patients were randomized to either mealtime FIASP or to mealtime NovoLog, both in combination with insulin glargine and metformin in a basal-bolus regimen. Mealtime FIASP or mealtime NovoLog was injected 0-2 minutes before the meal.

The mean age of the randomized subjects was 59.5 years and the mean duration of diabetes was 12.7 years. 49% were male, 81% were White, and 6% were Black or African American; and 6% were Hispanic or Latino. The mean BMI was 31.2 kg/m².

After 26 weeks of treatment, the treatment difference in HbA_{1c} reduction from baseline

between mealtime FIASP and mealtime NovoLog, both in combination with insulin glargine and metformin, met the pre-specified non-inferiority margin (0.4%). See Table 9. Insulin doses were similar among study arms at the end of the trial.

Table 9. Results from Study B: 26-Week Trial of Mealtime FIASP Compared to Mealtime NovoLog, Both used in Combination with Insulin Glargine and Metformin, in Adults with Type 2 Diabetes Mellitus

	Mealtime FIASP +insulin glargine +metformin	Mealtime NovoLog +insulin glargine +metformin
Number of subjects randomized (N)	345	344
HbA_{1c} (%)		
Baseline	8.0	7.9
Adjusted change from baseline	-1.38	-1.36
Estimated treatment difference vs. NovoLog [95%CI]*	-0.02 [-0.15;0.10]	

Baseline is based on the mean of the observed last available values prior to randomization.

*Tested for non-inferiority

Estimated treatment difference was calculated using mixed model for repeated measurements (MMRM).

11.9% of subjects on the Mealtime FIASP arm and 10.2% of subjects on the Mealtime NovoLog arm were missing the final HbA_{1c} assessment.

Study C (NCT01850615): FIASP added to basal insulin and metformin in patients with Type 2 Diabetes Mellitus inadequately controlled at baseline on basal insulin and metformin

The efficacy of FIASP was evaluated in an 18-week randomized, open-label, parallel group trial in 236 adult patients with type 2 diabetes mellitus who were inadequately controlled on basal insulin and metformin therapy, either with or without other oral antidiabetic therapy, for at least 3 months. Patients were randomized to either mealtime FIASP in addition to basal insulin and metformin or to continuing basal insulin and metformin therapy without FIASP. The basal insulins used in both treatment arms were insulin glargine, insulin detemir or NPH. All patients were also required to be on ≥ 1000 mg metformin treatment at baseline.

The mean age of the trial population was 57.4 years and the mean duration of diabetes was 11years. 48% were male, 70% were White and 4% were Black or African American; and 37% were Hispanic or Latino. The mean BMI was 30.8 kg/m².

After 18 weeks of treatment, addition of FIASP to basal insulin and metformin statistically significantly reduced HbA_{1c} compared to continuing basal insulin and metformin therapy without addition of FIASP (Table 10).

Table 10. Results from Study C: 18-Week Trial of Mealtime FIASP in Adults with Type 2 Diabetes Mellitus Inadequately Controlled at Baseline on Basal Insulin and Metformin

	FIASP + basal insulin + metformin	Basal insulin + metformin
Number of subjects randomized (N)	116	120
HbA_{1c} (%)		
Baseline	7.9	7.9
Adjusted change from baseline	-1.16	-0.22
Estimated treatment difference vs. basal insulin+metformin [95%CI]	-0.94 [-1.17; -0.72]*	
Proportion of patients Achieving HbA_{1c} < 7% at Trial End	60.3%	18.3%

Baseline is based on the mean of the observed last available values prior to randomization.

*p<0.0001, 1-sided p-value evaluated at 2.5% level for superiority.

Estimated treatment difference was calculated using mixed model for repeated measurements (MMRM).

6.0% of subjects on the mealtime FIASP arm and 3.3% of subjects on the placebo arm were missing the final HbA_{1c} assessment.

14.5 Type 1 Diabetes Mellitus- Adult Continuous Subcutaneous Insulin Infusion (CSII)

Study D (NCT02825251): FIASP in Continuous Subcutaneous Insulin Infusion (CSII) in Adults with Type 1 Diabetes Mellitus

The efficacy and safety of FIASP vs. NovoLog in CSII in adult subjects with type 1 diabetes mellitus (N=472) was evaluated in a randomized, multicenter, multinational, active controlled, treat-to-target, parallel group trial with a 4-week run-in and a 16-week treatment period. Meal-time bolus insulin infusion was initiated 0-2 minutes before a meal.

The mean age of the randomized subjects was 43 years and the mean duration of diabetes was 24 years. 43% were male. 89% were White, 1% were Black or African American, and 1% were Asian; and 3% were Hispanic or Latino. The mean BMI was 26.3 kg/m².

After 16 weeks of treatment, the treatment difference in HbA_{1c} reduction from baseline between FIASP and NovoLog was 0.10 with 95%CI [0.02, 0.18] (Table 11).

Table 11. Results from Study D: 16-Week Trial FIASP in Adults with Type 1 Diabetes

	FIASP	NovoLog
Number of subjects randomized (N)	236	236
HbA_{1c} (%)		
Baseline	7.5	7.5
Adjusted change from baseline	-0.04	-0.14
Estimated treatment difference FIASP vs. NovoLog [95%CI]*	0.10 [0.02; 0.18]	
Proportion of patients Achieving HbA_{1c} < 7% at Trial End	20.3%	23.3%

Baseline is based on the mean of the observed last available values prior to randomization.

*Tested for non-inferiority using a margin of 0.4%.

Estimated treatment difference was calculated using ANCOVA.

2.1% of subjects on the FIASP arm and 2.5% of subjects on the NovoLog arm were missing the final HbA_{1c} assessment. Missing values were imputed using multiple imputation with a mean equal to the baseline value of the corresponding patient.

16 HOW SUPPLIED/STORAGE AND HANDLING

16.1 How Supplied

FIASP (insulin aspart) injection 100 units of insulin aspart per mL (U-100) is available as a clear and colorless solution in the following presentations and packaging configurations:

Carton of one 10 mL multiple-dose vials NDC 0169-3201-11

Carton of five 3 mL single-patient-use FIASP FlexTouch pens NDC 0169-3204-15

Carton of five 3 mL single-patient-use PenFill cartridges* NDC 0169-3205-15

Carton of five 1.6 mL single-patient-use PumpCart cartridges** NDC 0169-3206-15

The FIASP FlexTouch pen dials in 1 unit increments.

* FIASP PenFill cartridges are designed for use with Novo Nordisk insulin delivery devices.

** FIASP PumpCart cartridges are designed for use in compatible pumps only.

16.2 Recommended Storage

Dispense in the original sealed carton with the enclosed Instructions for Use.

Unused FIASP vials should be stored between 2° to 8°C (36° to 46°F) in a refrigerator, but not in or near a freezing compartment. FIASP should not be exposed to excessive heat or light and must never be frozen. Do not use FIASP if it has been frozen. FIASP should **not** be drawn into a syringe and stored for later use.

Keep the cap on the pen in order to protect from light. Remove the needle from the FIASP FlexTouch pen after each injection and store without a needle attached. Use a new needle for each injection. Keep unused vials, FIASP FlexTouch, PenFill Cartridges and PumpCart cartridges in the carton so they will stay clean and protected from light.

The storage conditions for vials, FIASP FlexTouch pens, 3 mL PenFill cartridges and 1.6 mL PumpCart cartridges are summarized in Table 12:

Table 12. Storage Conditions for Vial, FIASP FlexTouch, PenFill Cartridges and PumpCart Cartridges

FIASP presentation	Not in-use (unopened)		In-use (opened)	
	Room Temperature (up to 30°C [86°F])	Refrigerated (2°C to 8°C [36°F to 46°F])	Room Temperature (up to 30°C [86°F])	Refrigerated (2°C to 8°C [36°F to 46°F])
10 mL multiple-dose vial	28 days	Until expiration date	28 days* (up to 30°C [86°F])	28 days*
3 mL single-patient-use FIASP FlexTouch pen	28 days	Until expiration date	28 days (up to 30°C [86°F])	28 days
3 mL single-patient-use PenFill cartridges	28 days	Until expiration date	28 days (up to 30°C [86°F])	Do not refrigerate
1.6 mL single-patient-use PumpCart cartridges	18 days**	Until expiration date	4 days** (up to 37°C [98.6°F])	Do not refrigerate

*Pump Reservoir: The total in use time is 28 days, including 6 days in the pump reservoir

**PumpCart Cartridges: The maximum time at room temperature is 18 days including 4 days in the pump

Storage of FIASP in Insulin Pump:

- Change FIASP in the pump reservoir at least every 6 days or according to the pump user manual, whichever is shorter.
- Replace the FIASP PumpCart cartridge at least every 4 days or according to the pump user manual, whichever is shorter.

- Change FIASP to avoid insulin degradation or after exposure to temperatures that exceed 37°C (98.6°F).
- The infusion set and infusion set insertion sites should be changed according to the manufacturers' user manual.

Storage of FIASP in Intravenous Infusion Fluids:

Infusion bags prepared as indicated under *Dosage and Administration (2.2)* are stable at room temperature at 20°C to 25°C (68°F to 77°F) for 24 hours.

17 PATIENT COUNSELING INFORMATION

Advise the patient to read the FDA-Approved Patient Labeling (Patient Information and Instructions for Use).

Never Share a FIASP FlexTouch Pen Device, PenFill Cartridge or PenFill Cartridge Device Between Patients

Advise patients that they should never share a FIASP FlexTouch pen device, PenFill cartridge or PenFill cartridge devices with another person, even if the needle is changed, because doing so carries a risk for transmission of blood-borne pathogens. Advise patients using FIASP vials not to share needles or syringes with another person. Sharing poses a risk for transmission of blood-borne pathogens [*see Warnings and Precautions (5.1)*].

Hyperglycemia or Hypoglycemia

Inform patients that hypoglycemia is the most common adverse reaction with insulin. Instruct patients on self-management procedures including glucose monitoring, proper injection technique, and management of hypoglycemia and hyperglycemia, especially at initiation of FIASP therapy. Instruct patients on handling of special situations such as intercurrent conditions (illness, stress, or emotional disturbances), an inadequate or skipped insulin dose, inadvertent administration of an increased insulin dose, inadequate food intake, and skipped meals. Instruct patients on the management of hypoglycemia [*see Warnings and Precautions (5.3)*].

Inform patients that their ability to concentrate and react may be impaired as a result of hypoglycemia. Advise patients who have frequent hypoglycemia or reduced or absent warning signs of hypoglycemia to use caution when driving or operating machinery.

Advise patients that changes in insulin regimen can predispose to hyperglycemia or hypoglycemia and that changes in insulin regimen should be made under close medical supervision [*see Warnings and Precautions (5.2)*].

Hypersensitivity Reactions

Advise patients that hypersensitivity reactions have occurred with FIASP. Inform patients on the symptoms of hypersensitivity reactions [*see Warnings and Precautions (5.6)*].

Hypoglycemia due to Medication Errors

Instruct patients to always check the insulin label before each injection to avoid mix-ups between insulin products.

Patients Using Continuous Subcutaneous Insulin Pumps

- Train patients in intensive insulin therapy with multiple injections and in the function of their pump and pump accessories.
- Instruct patients to follow healthcare provider recommendations when setting basal and meal time infusion rate.
- Refer to the continuous subcutaneous infusion pump user manual to see if FIASP can be used with the pump. See recommended reservoir and infusion sets in the insulin pump user manual.
- Instruct patients to change FIASP in the pump reservoir at least every 6 days, or replace the PumpCart cartridge at least every 4 days or according to the pump user manual, whichever is shorter; infusion sets and infusion set insertion sites should be changed in accordance with the manufacturers' user manual. By following this schedule, patients avoid insulin degradation, infusion set occlusion, and loss of the insulin preservative.
- Instruct patients to discard insulin exposed to temperatures higher than 37°C (98.6°F).
- Instruct patients to inform physician and select a new site for infusion if infusion site becomes erythematous, pruritic, or thickened.
- Instruct patients on the risk of rapid hyperglycemia and ketosis due to pump malfunction, infusion set occlusion, leakage, disconnection or kinking, and degraded insulin. Instruct patients on the risk of hypoglycemia from pump malfunction. If these problems cannot be promptly corrected, instruct patients to resume therapy with subcutaneous insulin injection and contact their physician [see *Warnings and Precautions (5) and How Supplied/Storage and Handling (16.2)*].

Version: 8

Novo Nordisk®, *FIASP®*, *NovoLog®*, *FlexTouch®*, *PenFill®* and *PumpCart®* are registered trademarks of Novo Nordisk A/S.

PATENT Information: <http://novonordisk-us.com/products/product-patents.html>

© 2023

Manufactured by:

Novo Nordisk Inc.
800 Scudders Mill Road
Plainsboro, New Jersey 08536
U.S. License 1261

For information about FIASP contact:

Novo Nordisk Inc.
800 Scudders Mill Road
Plainsboro, New Jersey 08536
1-800-727-6500

www.novonordisk-us.com

Patient Information

FIASP® (fee' asp)
(insulin aspart)

Injection, for subcutaneous or intravenous use

Do not share your FIASP with other people, even if the needle has been changed. You may give other people a serious infection, or get a serious infection from them.

What is FIASP?

- FIASP is a man-made insulin that is used to control high blood sugar in adults and children with diabetes mellitus.

Who should not take FIASP?

Do not take FIASP if you:

- are having an episode of low blood sugar (hypoglycemia).
- have an allergy to insulin aspart or any of the ingredients in FIASP.

Before taking FIASP, tell your healthcare provider about all your medical conditions including, if you:

- have kidney problems.
- have liver problems.
- are pregnant or plan to become pregnant. Talk with your healthcare provider about the best way to control your blood sugar if you plan to become pregnant or while you are pregnant.
- are breastfeeding or plan to breastfeed. It is not known if FIASP passes into your breast milk. Talk with your healthcare provider about the best way to feed your baby while using FIASP.
- are taking new prescription or over-the-counter medicines, vitamins, or herbal supplements.

Before you start taking FIASP, talk to your healthcare provider about low blood sugar and how to manage it.

How should I take FIASP?

- **Read the Instructions for Use** that come with your FIASP.
- Take FIASP exactly as your healthcare provider tells you to.
- **FIASP starts acting fast.** You should take your dose of FIASP at the beginning of the meal or within 20 minutes after starting a meal.
- Know the type and strength of insulin you take. **Do not** change the type of insulin you take unless your healthcare provider tells you to. The amount of insulin and the best time for you to take your insulin may need to change if you take different types of insulin.
- If you miss a dose of FIASP, monitor your blood sugar levels to decide if an insulin dose is needed. Continue with your regular dosing schedule at the next meal.
- **Check your blood sugar levels.** Ask your healthcare provider what your blood sugars should be and when you should check your blood sugar levels.
- **Do not reuse or share needles with other people. You may give other people a serious infection or get a serious infection from them.**
- FIASP can be injected under the skin (subcutaneously) of your stomach area, upper legs, or upper arms, or by continuous infusion under the skin (subcutaneously)

through an insulin pump into an area of your body recommended in the instructions that come with your insulin pump.

- **Change (rotate) your injection sites within the area you choose with each dose** to reduce your risk of getting pits in skin or thickened skin (lipodystrophy) and skin with lumps (localized cutaneous amyloidosis) at the injection sites.
 - o **Do not** use the exact same spot for each injection.
 - o **Do not** inject where the skin has pits, is thickened, or has lumps.
 - o **Do not** inject where the skin is tender, bruised, scaly or hard, or into scars or damaged skin.

What should I avoid while taking FIASP?

While taking FIASP do not:

- Drive or operate heavy machinery until you know how FIASP affects you.
- Drink alcohol or use prescription or over-the-counter medicines that contain alcohol.

What are the possible side effects of FIASP?

FIASP may cause serious side effects that can lead to death, including:

- **low blood sugar (hypoglycemia).** Signs and symptoms that may indicate low blood sugar include:

o dizziness or light-headedness	o blurred vision	o anxiety, irritability, or mood changes
o sweating	o slurred speech	o hunger
o confusion	o shakiness	o headache
o fast heart beat		

- **low potassium in your blood (hypokalemia).**
- **serious allergic reactions (whole body reactions).** Get emergency medical help right away, if you have any of these signs or symptoms of a severe allergic reaction:
 - o a rash over your whole body, trouble breathing, a fast heartbeat, swelling of your face, tongue or throat, sweating, extreme drowsiness, dizziness, confusion.
- **heart failure.** Taking certain diabetes pills called TZDs (thiazolidinediones) with FIASP may cause heart failure in some people. This can happen even if you have never had heart failure or heart problems before. If you already have heart failure it may get worse while you take TZDs with FIASP. Your healthcare provider should

monitor you closely while you are taking TZDs with FIASP. Tell your healthcare provider if you have any new or worse symptoms of heart failure including shortness of breath, swelling of your ankles or feet, sudden weight gain. Treatment with TZDs and FIASP may need to be adjusted or stopped by your healthcare provider if you have new or worse heart failure.

Your insulin dose may need to change because of:

<ul style="list-style-type: none">• change in level of physical activity or exercise	<ul style="list-style-type: none">• increased stress
<ul style="list-style-type: none">• change in diet	<ul style="list-style-type: none">• weight gain or loss
<ul style="list-style-type: none">• illness	

Common side effects of FIASP may include:

- skin problems such as eczema, rash, itching, redness and swelling of your skin (dermatitis)
- reactions at the injection site such as itching, rash
- skin thickening or pits at the injection site (lipodystrophy)
- weight gain

These are not all the possible side effects of FIASP. Call your doctor for medical advice about side effects. You may report side effects to FDA at 1-800-FDA-1088.

General information about the safe and effective use of FIASP.

Medicines are sometimes prescribed for purposes other than those listed in a Patient Information leaflet. You can ask your pharmacist or healthcare provider for information about FIASP that is written for health professionals. Do not use FIASP for a condition for which it was not prescribed. Do not give FIASP to other people, even if they have the same symptoms that you have. It may harm them.

What are the ingredients in FIASP?

Active Ingredient: insulin aspart

Inactive Ingredients: arginine, dibasic sodium phosphate, glycerin, metacresol, niacinamide, phenol, zinc and water for injection.

Manufactured by:

Novo Nordisk Inc.

U.S. License Number 1261

For more information, go to www.novonordisk-us.com or call 1-800-727-6500.

This Patient Information has been approved by the U.S. Food and Drug Administration.

Revised: 06/2023

INSTRUCTIONS FOR USE

FIASP (fee' asp)

(insulin aspart) injection

10 mL multiple-dose vial (100 units/mL, U-100)

Read this Instructions for Use before you start taking FIASP and each time you get a refill. There may be new information. This information does not take the place of talking to your healthcare provider about your medical condition or your treatment. The vial is not recommended for use by the blind or visually impaired without the assistance of a person trained in the proper use of the product and insulin syringe.

Do not reuse or share syringes or needles with other people. You may give other people a serious infection or get a serious infection from them.

Supplies you will need to give your FIASP injection:

- a 10 mL FIASP vial
- a U-100 insulin syringe and needle
- 2 alcohol swabs
- 1 sharps container for throwing away used needles and syringes. See “Disposing of your used needles and syringes” at the end of these instructions.






Preparing your FIASP dose:

- **Do not** roll or shake the FIASP vial. Shaking the FIASP vial right before the dose is drawn into the syringe may cause bubbles or foam. This can cause you to draw up the wrong dose of insulin.
- The tamper-resistant cap should not be loose or damaged before the first use. **Do not** use if the tamper-resistant cap is loose or damaged before using FIASP for the first time.
- Wash your hands with soap and water.
- **Before you start to prepare your injection, check the FIASP label to make sure that you are taking the right type of insulin. This is especially important if you use more than 1 type of insulin.**
- Check that the FIASP vial is not cracked or damaged. **Do not** use if the FIASP vial is cracked or damaged.

- FIASP should look clear and colorless. **Do not** use FIASP if it is thick, cloudy, or is colored.
- **Do not** use FIASP past the expiration date printed on the label.



<p>Step 1: Pull off the tamper-resistant cap (See Figure A).</p> <p>Step 2: Wipe the rubber stopper with an alcohol swab (See Figure B).</p>	 <p>(Figure A Figure B)</p>
<p>Step 3: Hold the syringe with the needle pointing up. Pull down on the plunger until the tip of the plunger reaches the line for the number of units for your prescribed dose (See Figure C).</p>	 <p>(Figure C)</p>
<p>Step 4: Push the needle through the rubber stopper of the FIASP vial (See Figure D).</p>	 <p>(Figure D)</p>
<p>Step 5: Push the plunger all the way in. This puts air into the FIASP vial (See Figure E).</p>	 <p>(Figure E)</p>
<p>Step 6: Turn the FIASP vial and syringe upside down and slowly pull the plunger down until the tip of the plunger is a few units past the line for your dose (See Figure F). If there are air bubbles, tap the syringe</p>	 <p>(Figure F)</p>

gently a few times to let any air bubbles rise to the top (See Figure G).



(Figure G)


Step 7: Slowly push the plunger up until the tip of the plunger reaches the line for your prescribed FIASP dose (See Figure H).



(Figure H)

Step 8: Check the syringe to make sure you have the right dose of FIASP.

Step 9: Pull the syringe out of the rubber stopper on the vial (See Figure I).



(Figure I)

Giving your FIASP injection:

- Inject your FIASP exactly as your healthcare provider has shown you. Your healthcare provider should tell you if you need to pinch the skin before injecting.
- You should take your dose of FIASP at the start of a meal or within 20 minutes after starting a meal.
- FIASP can be injected under the skin (subcutaneously) of your stomach area, upper legs, or upper arms, infused in an insulin pump into an area of your body recommended in the instructions that come with your insulin pump, or given through a needle in your arm (intravenously) by your healthcare provider. **Do not** inject FIASP into your muscle.
- If you use FIASP in an insulin pump, you should change the infusion sets and the infusion set insertion site according to the pump manufacturers' user manual. The insulin in the reservoir should be changed at least every 6 days even if you have not used all of the insulin.
- If you use FIASP in an insulin pump, see your insulin pump manual for instructions or talk to your healthcare provider. Your healthcare provider should provide recommendations for appropriate basal and meal time infusion rates.
- Change (rotate) your injection sites within the area you choose for each dose to reduce your risk of getting lipodystrophy (pits in skin or thickened skin) and localized cutaneous amyloidosis (skin with lumps) at the injection sites. **Do not** use the same injection site for each injection. **Do not** inject where the skin has pits, is thickened, or has lumps. **Do not** inject where the skin is tender, bruised, scaly or hard, or into scars or damaged skin.

- **Do not** dilute or mix FIASP with any other type of insulin products or solutions.

<p>Step 10: Choose your injection site (thighs, upper arms, or abdomen) and wipe the skin with an alcohol swab (See Figure J). Let the injection site dry before you inject your dose.</p>	 <p>(Figure J)</p>
<p>Step 11: Insert the needle into your skin. Push down on the plunger to inject your dose (See Figure K). Make sure you have injected all the insulin in the syringe.</p>	 <p>(Figure K)</p>
<p>Step 12: Pull the needle out of your skin. After your injection you may see a drop of FIASP at the needle tip. This is normal and does not affect the dose you just received (See Figure L).</p> <ul style="list-style-type: none"> • If you see blood after you take the needle out of your skin, press the injection site lightly with a piece of gauze or an alcohol swab. Do not rub the area. 	 <p>(Figure L)</p>

After your injection:

- **Do not** recap the needle. Recapping the needle can lead to needle stick injury.

Disposing of your used needles and syringes:

Put your used insulin needles and syringes in a FDA-cleared sharps disposal container right away after use. Do not throw away (dispose of) loose needles and syringes in your household trash.

If you do not have a FDA-cleared sharps disposal container, you may use a household container that is:

- o made of a heavy-duty plastic;
- o can be closed with a tight-fitting, puncture-resistant lid, without sharps being able to come out;
- o upright and stable during use;
- o leak-resistant, and
- o properly labeled to warn of hazardous waste inside the container.
- When your sharps disposal container is almost full, you will need to follow your community guidelines for the right way to dispose of your sharps disposal container. There may be state or local laws about how you should throw away used needles and syringes. Do not reuse or share needles or syringes with another person. For more information about safe sharps disposal, and for specific information about sharps disposal in the state that you live in, go to the FDA's

website at: <http://www.fda.gov/safesharpsdisposal>.

- Do not dispose of your used sharps disposal container in your household trash unless your community guidelines permit this. Do not recycle your used sharps disposal container.

How should I store FIASP?

- **Do not** freeze FIASP. **Do not** use FIASP if it has been frozen.
- Keep FIASP away from excessive heat or light.

All unopened vials:

- Store unopened FIASP vials in the refrigerator at 36°F to 46°F (2°C to 8°C) or at room temperature below 86°F (30°C).
- If unopened vials have been stored in the refrigerator, vials may be used until the expiration date printed on the label.
- If unopened vials have been stored at room temperature, vials should be thrown away after 28 days.

After vials have been opened:

- Opened FIASP vials can be stored in the refrigerator at 36°F to 46°F (2°C to 8°C) or at room temperature below 86°F (30°C).
- Throw away all opened FIASP vials after 28 days (including 6 days pump in-use time), even if they still have insulin left in them.

General information about the safe and effective use of FIASP

- Always use a new syringe and needle for each injection to help ensure sterility and prevent blocked needles.
- **Do not** reuse or share syringes or needles with other people. You may give other people a serious infection or get a serious infection from them.
- Keep FIASP vials, syringes, and needles out of the reach of children.

This Instructions for Use has been approved by the U.S. Food and Drug Administration.

Manufactured by:

Novo Nordisk Inc.

800 Scudders Mill Road

Plainsboro, NJ 08536

1-800-727-6500

U.S. License No. 1261

FIASP® is a registered trademark of Novo Nordisk A/S.

PATENT Information: <http://novonordisk-us.com/products/product-patents.html>

© 2023 Novo Nordisk

For information about FIASP® contact:

Novo Nordisk Inc.

800 Scudders Mill Road
Plainsboro, New Jersey 08536
1-800-727-6500
www.novonordisk-us.com
Revised: 06/2023

INSTRUCTIONS FOR USE

FIASP® [fee' asp]FlexTouch®

(insulin aspart)

injection, for subcutaneous use

3 mL single-patient-use pen: 100 units/mL (U-100)

- **Do not** share your FIASP FlexTouch Pen with other people, even if the needle is changed. You may give other people a serious infection, or get a serious infection from them.
- **FIASP FlexTouch Pen (“Pen”) is a prefilled disposable, single-patient-use pen** containing 300 units of U-100 FIASP (insulin aspart) injection. You can inject from 1 to 80 units in a single injection. The units can be increased by 1 unit at a time.
- People who are blind or have vision problems should not use the Pen without help from a person trained to use the Pen.
- **Do not** use a syringe to remove FIASP from the FlexTouch Pen.


Supplies you will need to give your FIASP injection:

- FIASP FlexTouch Pen
- a new NovoFine, NovoFine Plus or NovoTwist needle
- alcohol swab
- a sharps container for throwing away used Pens and needles. **See “After your injection” at the end of these instructions.**


Preparing your FIASP FlexTouch Pen:

- Wash your hands with soap and water.
- Before you start to prepare your injection, check the FIASP FlexTouch Pen label to make sure you are taking the right type of insulin. This is especially important if you take more than 1 type of insulin.
- FIASP should look clear and colorless. **Do not** use FIASP if it is thick, cloudy, or is colored.
- **Do not** use FIASP past the expiration date printed on the label or 28 days after you start using the Pen.
- **Always** use a new needle for each injection to help ensure sterility and prevent blocked needles. **Do not** reuse or share needles with another person. You may give other people a serious infection, or get a serious infection from them.


NovoFine®

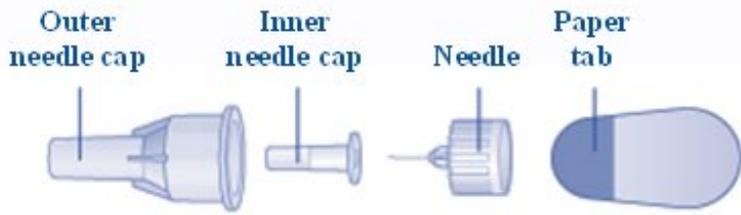






NovoFine® Plus

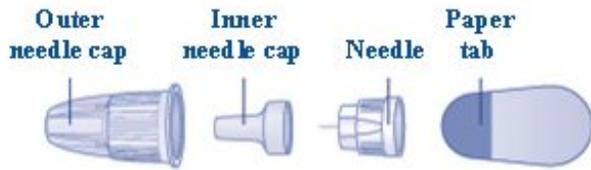

NovoTwist®

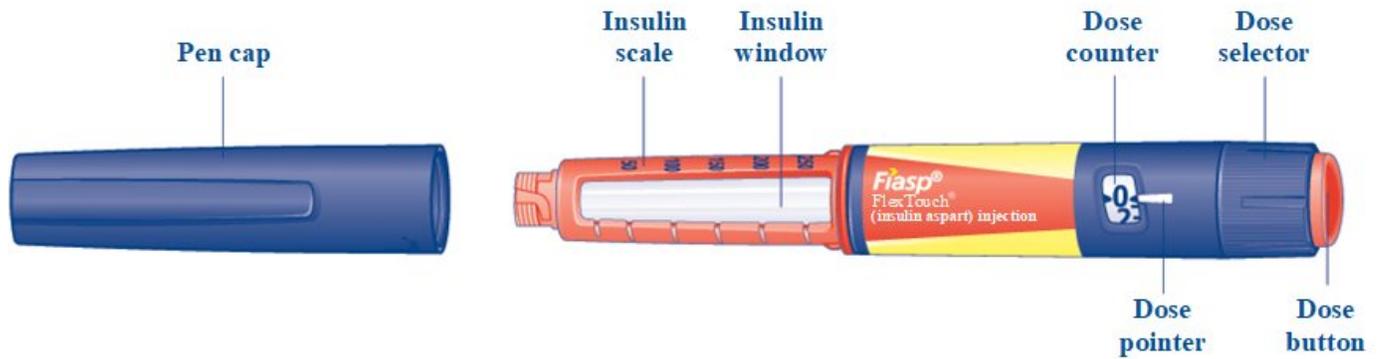

(Figure A)
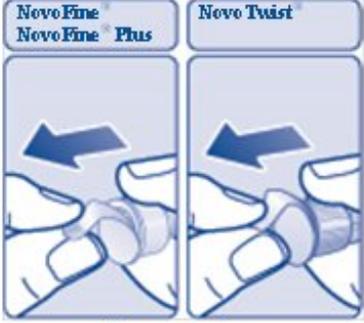
<p>Step 1:</p> <ul style="list-style-type: none"> • Pull Pen cap straight off (See Figure B). 	 <p>(Figure B)</p>
<p>Step 2:</p> <ul style="list-style-type: none"> • Check the liquid in the Pen (See Figure C). FIASP should look clear and colorless. Do not use it if it looks cloudy or colored. 	 <p>(Figure C)</p>
<p>Step 3:</p> <ul style="list-style-type: none"> • Select a new needle. • Pull off the paper tab from the outer needle cap (See Figure D). 	 <p>(Figure D)</p>
<p>Step 4:</p> <ul style="list-style-type: none"> • Push the capped needle straight onto the Pen and twist the needle on until it is tight (See Figure E). 	 <p>(Figure E)</p>
<p>Step 5:</p> <ul style="list-style-type: none"> • Pull off the outer needle cap. Do not throw it away (See Figure F). 	 <p>(Figure F)</p>
<p>Step 6:</p> <ul style="list-style-type: none"> • Pull off the inner needle cap and throw it away (See Figure G). 	 <p>(Figure G)</p>

Priming your FIASP FlexTouch Pen:

Step 7:


- Turn the dose selector to **select 2 units** (See Figure H).



(Figure H)

Step 8:


- Hold the Pen with the needle pointing up. Tap the top of the Pen gently a few times to let any air bubbles rise to the top (See Figure I).



(Figure I)

Step 9:

- **Hold the Pen with the needle pointing up.** Press and hold in the dose button until the dose counter shows "0". The "0" must line up with the dose pointer.
- A drop of insulin should be seen at the needle tip (See Figure J).
- o If you **do not** see a drop of insulin, repeat steps 7 to 9, no more than 6 times.
- o If you **still do not** see a drop of insulin, change the needle and repeat steps 7 to 9.

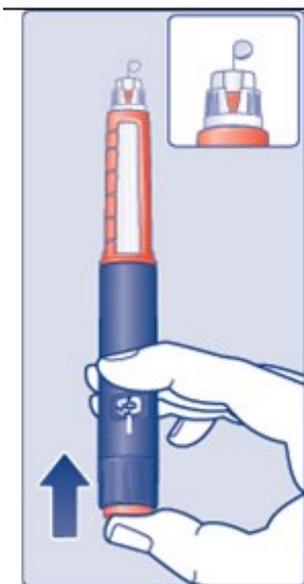


(Figure J)

Selecting your dose:


Step 10:
Check to make sure the dose selector is set at 0.

- **Turn the dose selector to select the number of units you need to inject.** The dose pointer should line up with your dose (See Figure K).
- o If you select the wrong dose, you can turn the dose selector forwards or backwards to the correct dose.
- o The **even** numbers are printed on the dial.
- o The **odd** numbers are shown as lines.

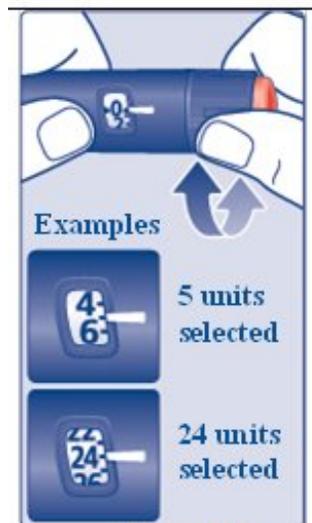

(Figure K)

- The FIASP FlexTouch Pen insulin scale will show you how much insulin is left in your Pen (See Figure L).

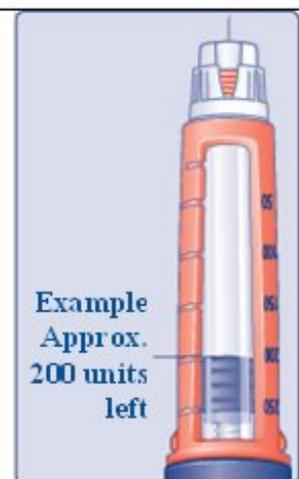




(Figure L)

- **To see how much insulin is left in your FIASP FlexTouch Pen:**
- o Turn the dose selector until it stops. The dose counter will line up with the number of units of insulin that is left in your Pen. If the dose counter shows 80, there are **at least 80** units left in your Pen.
- o If the dose counter shows **less than 80**, the number shown in the dose counter is the number of units left in your Pen.

Giving your injection:

- Inject your FIASP exactly as your healthcare provider has shown you. Your healthcare provider should tell you if you need to pinch the skin before injecting.
- You should take your dose of FIASP at the start of a meal or within 20 minutes after starting a meal.


- FIASP can be injected under the skin (subcutaneously) of your stomach area (abdomen), upper legs (thighs) or upper arms. **Do not** inject FIASP into your muscle.
- Change (rotate) your injection sites within the area you choose for each dose to reduce your risk of getting lipodystrophy (pits in skin or thickened skin) and localized cutaneous amyloidosis (skin with lumps) at the injection sites. **Do not** use the same injection site for each injection. **Do not** inject where the skin has pits, is thickened, or has lumps. **Do not** inject where the skin is tender, bruised, scaly or hard, or into scars or damaged skin.

<p>Step 11:</p> <ul style="list-style-type: none"> • Choose your injection site (thighs, upper arms, or abdomen) and wipe the skin with an alcohol swab. Let the injection site dry before you inject your dose (See Figure M). 	 <p>(Figure M)</p>
<p>Step 12:</p> <ul style="list-style-type: none"> • Insert the needle into your skin (See Figure N). <ul style="list-style-type: none"> ○ Make sure you can see the dose counter. Do not cover it with your fingers; this can stop your injection. 	 <p>(Figure N)</p>
<p>Step 13:</p> <ul style="list-style-type: none"> • Press and hold down the dose button until the dose counter shows “0” (See Figure O). <ul style="list-style-type: none"> ○ The “0” must line up with the dose pointer. You may then hear or feel a click. • Keep the needle in your skin after the dose counter has returned to “0” and slowly count to 6 (See Figure P). <ul style="list-style-type: none"> ○ When the dose counter returns to “0”, you will not get your full dose until 6 seconds later. ○ If the needle is removed before you count to 6, you may see a stream of insulin coming from the needle tip. ○ If you see a stream of insulin 	 <p>(Figure O)</p>  <p>(Figure P)</p>

coming from the needle tip you will not get your full dose. If this happens you should check your blood sugar levels more often because you may need more insulin.

Step 14:


- **Pull the needle out of your skin** (See Figure Q).
 - o If you see blood after you take the needle out of your skin, press the injection site lightly with a piece of gauze or an alcohol swab. **Do not** rub the area.




(Figure Q)

Step 15:

- **Carefully remove the needle from the Pen and throw it away** (See Figure R).
 - o **Do not** recap the needle. Recapping the needle can lead to needle stick injury.
- If you **do not** have a sharps container, carefully slip the needle into the outer needle cap (See Figure S). Safely remove the needle and throw it away as soon as you can.
 - o **Do not** store the Pen with the needle attached. Storing without the needle attached helps prevent leaking, blocking of the needle, and air from entering the Pen.




(Figure R)



(Figure S)

Step 16:

- Replace the Pen cap by pushing it straight on (See Figure T).



(Figure T)

After your injection:

- Put your used needles in a FDA-cleared sharps disposal container right away after use. Do not throw away (dispose of) loose needles in your household trash.
- If you do not have a FDA-cleared sharps disposal container, you may use a household container that is:
 - o made of a heavy-duty plastic
 - o can be closed with a tight-fitting, puncture-resistant lid, without sharps being able to come out
 - o upright and stable during use
 - o leak-resistant
 - o properly labeled to warn of hazardous waste inside the container
- When your sharps disposal container is almost full, you will need to follow your community guidelines for the right way to dispose of your sharps disposal container. There may be state or local laws about how you should throw away used needles and syringes. Do not reuse or share needles or syringes with another person. For more information about safe sharps disposal, and for specific information about sharps disposal in the state that you live in, go to the FDA's website at: <http://www.fda.gov/safesharpsdisposal>.
- Do not dispose of your used sharps disposal container in your household trash unless your community guidelines permit this. Do not recycle your used sharps disposal container.

How should I store my FIASP FlexTouch Pen?

Before use:

- Store unused FIASP FlexTouch Pens in the refrigerator at 36°F to 46°F (2°C to 8°C) or at room temperature below 86°F (30°C).
- **Do not** freeze FIASP. **Do not** use FIASP if it has been frozen.
- Unused Pens may be used until the expiration date printed on the label, if kept in the refrigerator.
- If FIASP FlexTouch Pens are stored at room temperature prior to first use, it should be used or thrown away within 28 days.

Pen in use:

- Store the Pen you are currently using without the needle attached at room temperature below 86°F (30°C) or in the refrigerator at 36°F to 46°F (2°C to 8°C) for up to 28 days.
- Keep FIASP away from excessive heat or light.
- The FIASP FlexTouch Pen you are using is to be thrown away after 28 days, even if it still has insulin left in it and the expiration date has not passed.

General Information about the safe and effective use of FIASP:

- **Keep FIASP FlexTouch Pens and needles out of the reach of children.**
- **Always** use a new needle for each injection.
- **Do not** share FIASP FlexTouch Pens or needles with other people. You may give other people a serious infection, or get a serious infection from them.

This Instructions for Use has been approved by the U.S. Food and Drug Administration.

Manufactured by:

Novo Nordisk Inc.

800 Scudders Mill Road

Plainsboro, NJ 08536

1-800-727-6500

U.S. License No. 1261

Revised: 06/2023



For more information go to

www.FIASPflectouch.com

© 2023 Novo Nordisk



INSTRUCTIONS FOR USE

FIASP® [fee'asp] PenFill®

(insulin aspart)

injection, for subcutaneous use

3 mL cartridge: 100 units/mL (U-100)


- **Do not share your PenFill cartridge or PenFill cartridge compatible insulin delivery device with other people, even if the needle has been changed. You may give other people a serious infection, or get a serious infection from them.**
- Your healthcare provider should show you or your caregiver how to inject FIASP the right way before you inject it for the first time.
- **FIASP PenFillcartridge 100 units/mL is a prefilled single-patient-use cartridge** containing 300 units of U-100 FIASP (insulin aspart) injection.
- After you insert the PenFill cartridge in your device, you can use it for multiple injections. Read the **instruction manual** that comes with your insulin delivery

device for complete instructions on how to use the PenFill cartridge with the device.

- This PenFill cartridge is not recommended for use by the blind or visually impaired without the assistance of a person trained in the proper use of the product and your insulin delivery device.
- If using a **new** FIASP PenFill cartridge, start with **Step 1**.
- If the FIASP PenFill cartridge has already been **used**, start with **Step 2**.

Supplies you will need to give your FIASP injection:

- FIASP PenFill cartridge
- Novo Nordisk 3 mL PenFill cartridge compatible insulin delivery device
- 1 new NovoFine[®], NovoFine[®] Plus, or NovoTwist[®] needle
- Alcohol swab
- Adhesive bandage
- Cotton gauze
- A sharps container for throwing away used PenFill cartridges and needles. **See “After your injection” at the end of these instructions.**

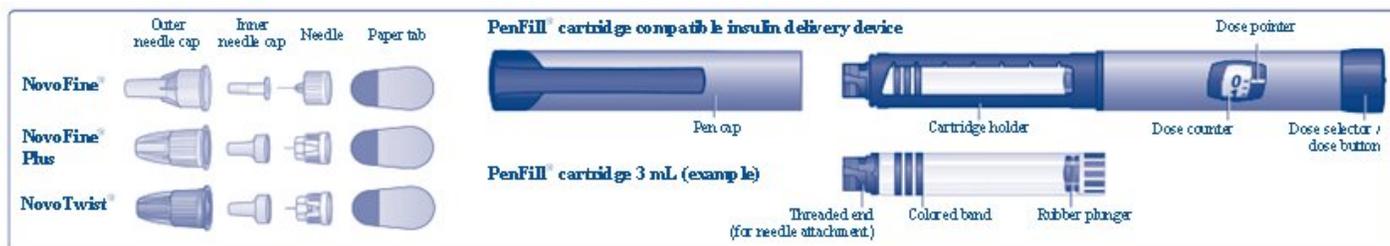

(Figure A)

How to use the FIASP PenFill cartridge

- Wash your hands with soap and water.
- Before you start to prepare your injection, **check the FIASP PenFill cartridge label** to make sure that it contains the insulin you need. This is especially important if you take more than 1 type of insulin.
- The tamper-resistant foil should be in place before the first use. If the foil has been broken or removed before your first use of the cartridge, **do not** use it. Call Novo Nordisk at 1-800-727-6500.
- Carefully look at the cartridge and the insulin inside it. Check that the FIASP cartridge:
 - o is not damaged, for example cracked or leaking
 - o is not loose on the threaded end
- FIASP should look clear and colorless. **Do not** use FIASP if it is cloudy or colored or if the threaded end is loose (See Figure B).



(Figure B)

Step 1:

- Insert a 3 mL cartridge with the threaded end first into your Novo Nordisk 3 mL PenFill cartridge compatible insulin delivery device (See Figure C).
- If you drop your device, check the insulin cartridge for damage such as cracks or leaking. If your cartridge is damaged, throw it away and use a new one.




(Figure C)

Prepare your device with a new needle

Step 2:


- **Take a new needle**, and tear off the paper tab. Always use a new needle for each injection to make sure the needle is free of germs (sterile) and to prevent blocked needles. **Do not attach a new needle** to your device until you are ready to give your injection. **Do not reuse or share your needles with other people. You may give others a serious infection, or get a serious infection from them.**
- Be careful not to bend or damage the needle before you use it.
- Push the needle straight onto the device. Turn the needle clockwise until it is on tight (See Figure D).

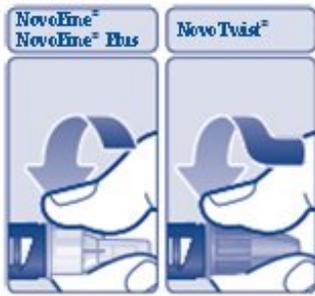

(Figure D)

Step 3:


- **Pull off the outer needle cap** (See Figure E). **Do not** throw it away. You will need it after the injection to safely remove the needle.

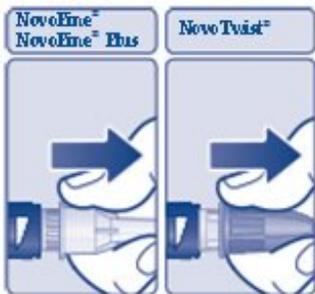

(Figure E)

Step 4:

- **Pull off the inner needle cap** and throw it away (See Figure F). **Do not** try to put the inner needle cap back on the needle.

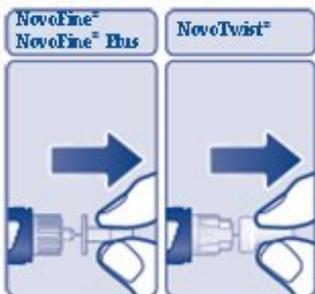

(Figure F)

A drop of insulin may appear at the needle tip. This is normal, but you must still check the insulin flow.

Check the insulin flow

Step 5:

- Small amounts of air may collect in the cartridge during normal use. You must do an airshot before each injection to avoid injecting air and to make sure you receive the prescribed dose of your medicine.
- Do the airshot as described in the instruction manual that comes with your device.
- Keep testing your Novo Nordisk 3 mL PenFill cartridge compatible insulin delivery device until you see insulin at the needle tip. If you still do not see a drop of insulin after 6 times, change the needle and repeat this step. This makes sure that any air bubbles are removed and that insulin is getting through the needle (See Figure G).




(Figure G)

Select your dose

Step 6:

- **Check to make sure that the dose counter is set to 0.**
- **Turn the dose selector clockwise to select the dose you need** to inject (See Figure H). The pointer should line up with your dose. When turning the dose selector, be careful not to press the dose button as insulin will come out. You will hear a click for every single unit dialed. **Do not** set the dose by counting the number of clicks you hear because you may get an incorrect dose.
- Refer to your insulin delivery device manual if necessary.

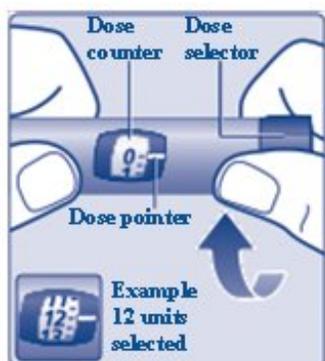


(Figure H)

Inject your dose


Step 7:

- **Do the injection exactly as shown to you by your healthcare provider. Your healthcare provider should tell you if you need to pinch the skin before injecting.**
- **You should take your dose of FIASP at the start of a meal or within 20 minutes after starting a meal.**
- **FIASP can be injected under the skin (subcutaneously) of your stomach area (abdomen), upper legs (thighs), or upper arms (See Figure I).**

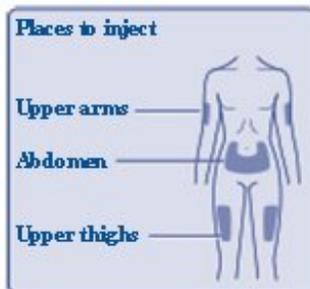

(Figure I)

- **Change (rotate) your injection sites within the area you choose for each dose to reduce your risk of getting lipodystrophy (pits in skin or thickened skin) and localized cutaneous amyloidosis (skin with lumps) at the injection sites. Do not use the same injection site for each injection. Do not inject where the skin has pits, is thickened, or has lumps. Do not inject where the skin is tender, bruised, scaly or hard, or into scars or damaged skin.**
- **Clean your injection site with an alcohol swab. Let your skin dry. Do not touch this area again before injecting.**
- **Insert the needle into your skin. Press and hold down the dose button until the dose counter shows "0". Continue to keep the dose button pressed and keep the needle in your skin and slowly count to 6 (see Figure J).**
- **Remove the needle from your skin.**

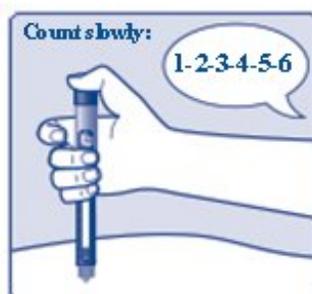

(Figure J)


You may see a drop of FIASP at the needle tip after injecting. This is normal and has no effect on the dose you just received. If blood appears after you take the needle out of

your skin, press the injection site lightly with a cotton gauze and cover with an adhesive bandage, if necessary. **Do not rub the area.**

After your injection

Step 8:

- Lay your outer needle cap on a flat surface. Carefully, lead the needle tip into the outer needle cap without touching the needle (See Figure K) and push the outer needle cap completely on.

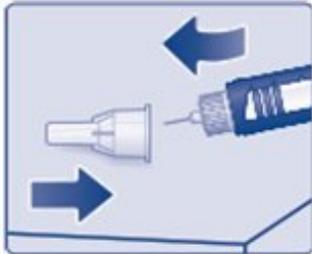

(Figure K)

- Hold the black cartridge holder on the insulin delivery device and unscrew the needle counterclockwise (See Figure L).




(Figure L)

- Throw away (dispose of) the needle in an FDA-cleared sharps container as your healthcare professional has instructed you.
- Put your empty FIASP PenFill cartridge and used needles in a FDA-cleared sharps disposal container right away after use. Do not throw away (dispose of) loose needles and PenFill cartridges in your household trash.
- If you do not have a FDA-cleared sharps disposal container, you may use a household container that is:
 - o made of a heavy-duty plastic
 - o can be closed with a tight-fitting, puncture-resistant lid, without sharps being able to come out
 - o upright and stable during use
 - o leak-resistant
 - o properly labeled to warn of hazardous waste inside the container

- When your sharps disposal container is almost full, you will need to follow your community guidelines for the right way to dispose of your sharps disposal container. There may be state or local laws about how you should throw away used needles and syringes. Do not reuse or share your needles or syringes with other people. For more information about the safe sharps disposal, and for specific information about sharps disposal in the state that you live in, go to the FDA's website at: <http://www.fda.gov/safesharpsdisposal>.
- Do not dispose of your used sharps disposal container in your household trash unless your community guidelines permit this. Do not recycle your used sharps disposal container.

Step 9:

- Keep the 3 mL PenFill cartridge in the device. **Do not** store your device with a needle attached. This will prevent infection or leakage of insulin and will make sure that you receive the right dose of FIASP.
- **Put the pen cap on** your device after each use to protect the insulin from light (See Figure M).

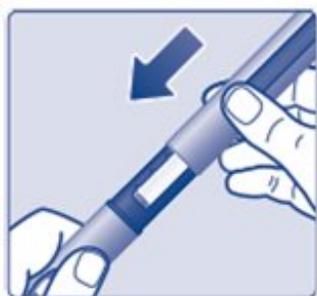

(Figure M)

How should I store my FIASP PenFill cartridge?

Before use:

- Store unused FIASP PenFill cartridges in the refrigerator at 36°F to 46°F (2°C to 8°C).
- **Do not** freeze FIASP. **Do not** use FIASP if it has been frozen.
- Unused PenFill cartridges may be used until the expiration date printed on the label, if kept in the refrigerator.
- If FIASP is stored mistakenly outside of refrigeration between 47°F (9°C) to 86°F (30°C) prior to first use, it should be used within 28 days or thrown away.

PenFill cartridges in use:

- Store the PenFill cartridge you are currently using in the insulin delivery device at room temperature below 86°F (30°C) for up to 28 days. Do not refrigerate.
- Keep FIASP away from heat or light.
- The FIASP PenFill cartridge you are using should be thrown away after 28 days, even if it still has insulin left in it.

General Information about the safe and effective use of FIASP.

- **Keep FIASP PenFill cartridges and needles out of the reach of children.**
- **Do not** share FIASP PenFill cartridges or needles with other people. You may give other people a serious infection, or get a serious infection from them.
- **Always carry extra insulin of the same type(s) you use in case of loss or damage.**

This Instructions for Use has been approved by the U.S. Food and Drug Administration.

© 2023 Novo Nordisk

Manufactured by:

Novo Nordisk Inc.

800 Scudders Mill Road

Plainsboro, NJ 08536

1-800-727-6500

U.S. License No. 1261

Revised: 06/2023

INSTRUCTIONS FOR USE


FIASP® [fee'asp] PumpCart®

(insulin aspart)

injection, for subcutaneous use

1.6 mL cartridge: 100 units/mL (U-100)

- **Please read the pump manual (user guide)** that comes with your insulin pump.
- Only use FIASP PumpCart with a compatible insulin pump. Check the insulin pump manual for instructions to see if FIASP PumpCart can be used with the pump. Do not use with other devices that are not designed for use with FIASP PumpCart.
- FIASP PumpCart is ready for use directly in the pump. Using the wrong device may result in the wrong insulin dosing and lead to high blood sugar (hyperglycemia) or low blood sugar (hypoglycemia).
- Do not share your PumpCart cartridge with other people. You may give other people a serious infection or get a serious infection from them.
- Do not use the PumpCart cartridge if you are blind or visually impaired without the assistance of a person trained in the proper use of the PumpCart.
- Do not mix with any other insulins.
- Do not refill FIASP PumpCart. When it is empty, throw away (dispose) the cartridge.
- Do not use FIASP PumpCart in an insulin pen.

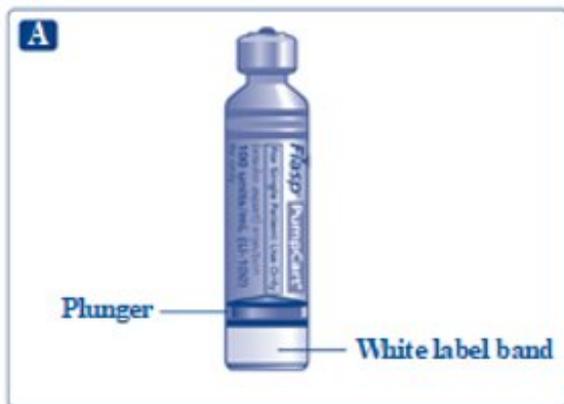

Preparing and Using the FIASP PumpCart cartridge

- Take FIASP PumpCart out of its package.
- Check the label to make sure that it is FIASP PumpCart and confirm that you are using a compatible insulin pump.
- Check the expiry date (EXP) – which is on the label and the carton.
- See picture A. **Do not use the cartridge** if any damage or leakage is seen, if the plunger has moved, or if the bottom of the plunger is visible above the white label band. This could be a result of leakage of insulin. Contact Novo Nordisk If you suspect that your FIASP PumpCart cartridge is damaged.
- Check that the insulin in FIASP PumpCart is clear and colorless. If the insulin looks cloudy, do not use FIASP PumpCart. The cartridge may contain small bubbles.
- Wash your hands with soap and water prior to installing the cartridge in your insulin pump.
- Follow the instructions in the pump user manual to insert a new FIASP PumpCart cartridge in your pump and to remove the FIASP PumpCart cartridge from your pump.
- Replace the FIASP PumpCart cartridge at least every 4 days, or according to the pump user manual, whichever is shorter, even if you have not used all of the insulin.
- Change the infusion sets and the infusion set insertion site according to the insulin pump manufacturers' user manual.
- Throw away FIASP PumpCart in the pump reservoir if it has been exposed to temperatures higher than 98.6°F (37°C).

How should I dispose my FIASP PumpCart cartridge?

- Put your empty FIASP PumpCart in a FDA-cleared sharps disposal container right away after use. Do not throw away (dispose of) Fiasp PumpCart in your household trash.
- If you do not have a FDA-cleared sharps disposal container, you may use a household container that is:
 - o made of a heavy-duty plastic
 - o can be closed with a tight-fitting, puncture-resistant lid, without sharps being able to come out
 - o upright and stable during use
 - o leak-resistant
 - o properly labeled to warn of hazardous waste inside the container

- When your sharps disposal container is almost full, you will need to follow your community guidelines for the right way to dispose of your sharps disposal container. There may be state or local laws about how you should throw away used needles and syringes. For more information about safe sharps disposal, and for specific information about sharps disposal in the state that you live in, go to the FDA's website at: <http://www.fda.gov/safesharpsdisposal>. Do not dispose of your used sharps disposal container in your household trash unless your community guidelines permit this. Do not recycle your used sharps disposal container.

How should I store my FIASP PumpCart cartridge?

- Not in-use (unopened) cartridges: Refrigerate at 36°F to 46°F (2°C to 8°C) in the original carton until expiration or for up to 18 days below 86°F (30°C).
- In-use (opened) cartridge: Do not refrigerate. Keep below 98.6°F (37°C) for up to 4 days. The maximum time at room temperature is 18 days including 4 days in the pump.
- Do not freeze.
- Keep FIASP PumpCart cartridge away from heat or light.

General Information about the safe and effective use of FIASP PumpCart cartridge

- Keep FIASP PumpCart out of the reach of children.
- Always carry extra insulin of the same type you use in case of loss or damage.

This Instructions for Use has been approved by the U.S. Food and Drug Administration.

© 2023 Novo Nordisk

Manufactured by:

Novo Nordisk Inc.

800 Scudders Mill Road

Plainsboro, New Jersey 08536

US License Number 1261

Revised: 06/2023

PRINCIPAL DISPLAY PANEL - VIAL

NDC 0169-3201-11 List 320111


FIASP®

(insulin apart) injection

100 units/mL (U-100)

For subcutaneous or intravenous use

Rx only **One 10 mL multi-dose vial**

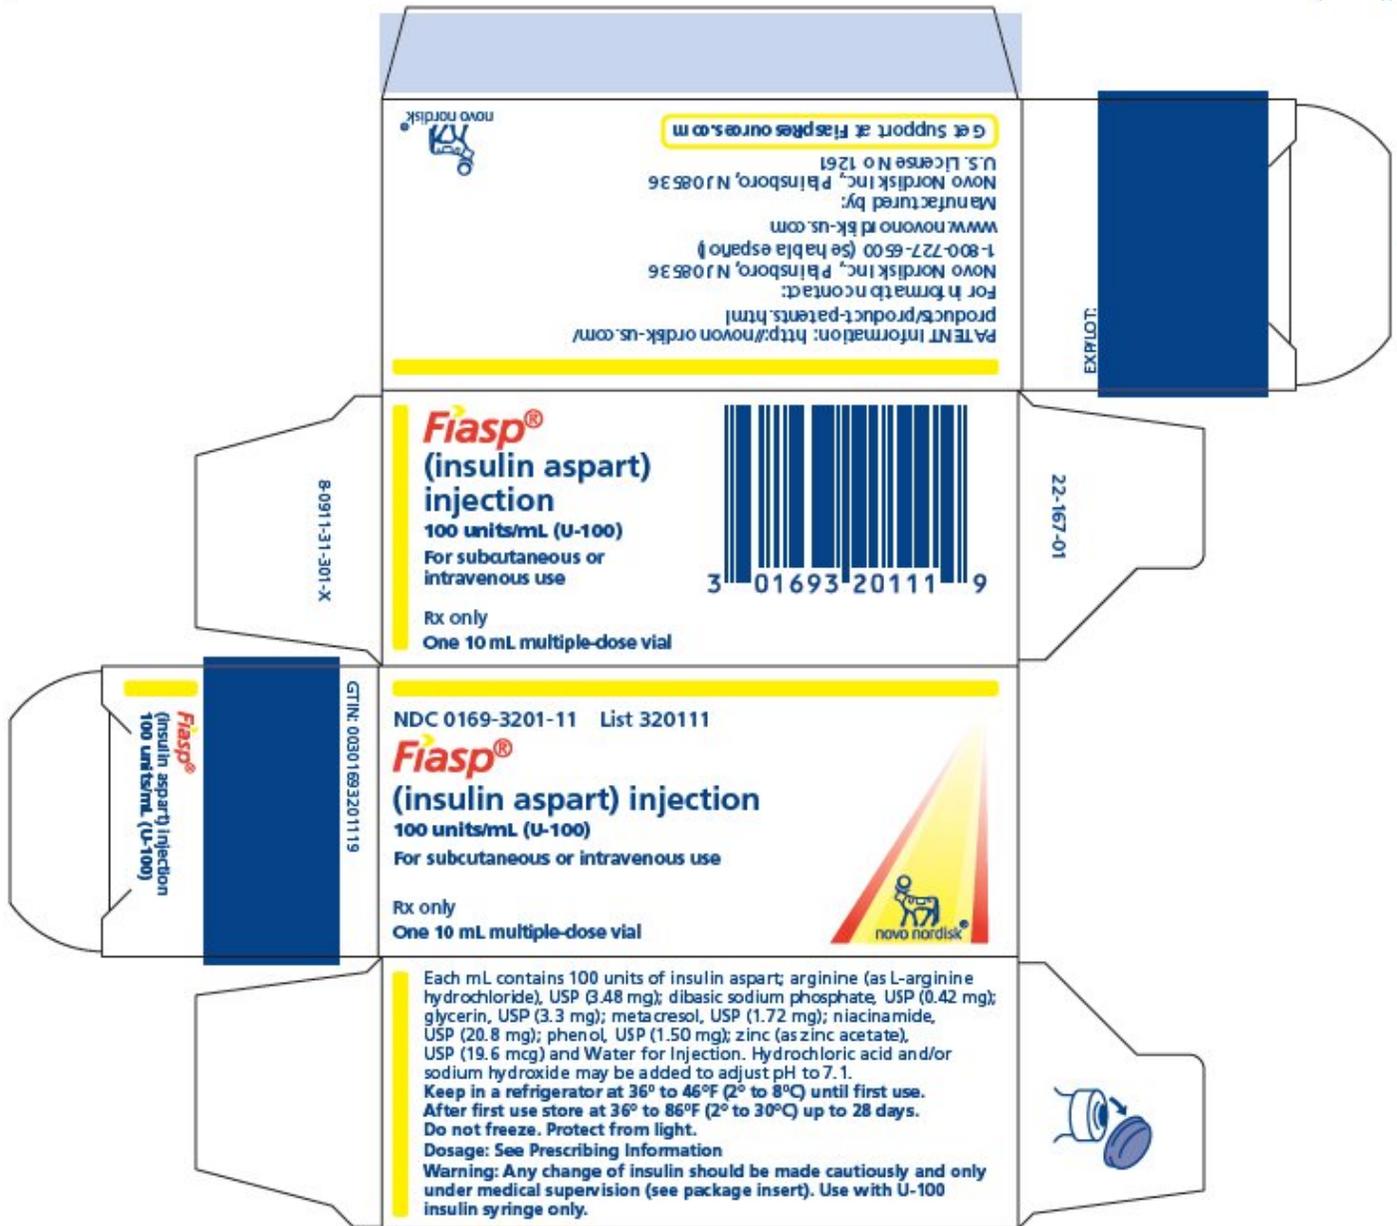

PRINCIPAL DISPLAY PANEL - FLEXTOUCH

NDC 0169-3204-15 List 320415

FIASP® FlexTouch®

(insulin aspart) injection

For Single-Patient Use Only

100 units/mL (U-100)

For subcutaneous use only

Rx Only

**Recommended for use with NovoFine® or
NovoFine® Plus disposable needles.**

Keep in a refrigerator at 36° to 46°F (2° to 8°C) until first use.

After first use store at 36° to 86°F (2° to 30°C) up to 28 days.

Do not freeze.

Protect from light.

Dispense in this sealed carton.

5×3 mL Prefilled Pens



PRINCIPAL DISPLAY PANEL - PenFill

NDC 0169-3205-15 List 320515

FIASP® PenFill®

(insulin aspart) injection

For Single-Patient Use Only

100 units/mL (U-100)

For Subcutaneous Use

For use with Novo Nordisk 3 mL PenFill® cartridge compatible delivery devices, NovoPen® Echo®, and NovoFine®/NovoFine® Plus disposable needles.

Not in-use (unopened) cartridges: Refrigerate at 36°F to 46°F (2°C to 8°C) in the original carton. In-use (opened) cartridge: Keep at room temperature below 86°F (30°C). Once stored at room temperature, discard after 28 days. Do not freeze. Protect from light.

Rx only

3 mL cartridges

5 cartridges per package



Principal Display Panel - PumpCart

NDC 0169-3206-15 List 320615

Fiasp[®] PumpCart[®]

(insulin aspart) injection

For Single-Patient Use Only

100 units/mL (U-100)

For use with a compatible insulin pump only

For Subcutaneous Use

Not in-use (unopened) cartridges: Refrigerate at 36°F to 46°F (2°C to 8°C) until expiration or for up to 18 days below 86°F (30°C) in the original carton.

In-use (opened) cartridges: Keep below 98.6°F (37°C) for up to 4 days.

Do not freeze. Protect from light.

Rx only

1.6 mL cartridges

5 cartridges per package



FIASP

insulin aspart injection injection, solution

Product Information

Product Type	HUMAN PRESCRIPTION DRUG	Item Code (Source)	NDC:0169-3201
Route of Administration	SUBCUTANEOUS		

Active Ingredient/Active Moiety

Ingredient Name	Basis of Strength	Strength
INSULIN ASPART (UNII: D933668QVX) (INSULIN ASPART - UNII:D933668QVX)	INSULIN ASPART	100 [iU] in 1 mL

Inactive Ingredients

Ingredient Name	Strength
WATER (UNII: 059QF0KO0R)	

Other Ingredients

Ingredient Kind	Ingredient Name	Quantity
May contain	HYDROCHLORIC ACID (UNII: QTT17582CB)	
May contain	SODIUM HYDROXIDE (UNII: 55X04QC32I)	

Packaging

#	Item Code	Package Description	Marketing Start Date	Marketing End Date
1	NDC:0169-3201-11	1 in 1 CARTON	10/20/2017	
1		10 mL in 1 VIAL, GLASS; Type 0: Not a Combination Product		
2	NDC:0169-3201-90	1 in 1 CARTON	10/20/2017	
2		10 mL in 1 VIAL, GLASS; Type 0: Not a Combination Product		

Marketing Information

Marketing Category	Application Number or Monograph Citation	Marketing Start Date	Marketing End Date
BLA	BLA208751	10/20/2017	

FIASP

insulin aspart injection injection, solution

Product Information

Product Type	HUMAN PRESCRIPTION DRUG	Item Code (Source)	NDC:0169-3204
Route of Administration	SUBCUTANEOUS		

Active Ingredient/Active Moiety

Ingredient Name	Basis of Strength	Strength
INSULIN ASPART (UNII: D933668QVX) (INSULIN ASPART - UNII:D933668QVX)	INSULIN ASPART	100 [iU] in 1 mL

Inactive Ingredients

Ingredient Name	Strength
SODIUM PHOSPHATE, DIBASIC, UNSPECIFIED FORM (UNII: GR686LBA74)	0.42 mg in 1 mL
WATER (UNII: 059QF0KO0R)	

Other Ingredients

Ingredient Kind	Ingredient Name	Quantity
-----------------	-----------------	----------

May contain	HYDROCHLORIC ACID (UNII: QTT17582CB)	
May contain	SODIUM HYDROXIDE (UNII: 55X04QC32I)	

Packaging

#	Item Code	Package Description	Marketing Start Date	Marketing End Date
1	NDC:0169-3204-15	5 in 1 CARTON	10/20/2017	
1		3 mL in 1 SYRINGE, PLASTIC; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		
2	NDC:0169-3204-97	1 in 1 CARTON	10/20/2017	
2	NDC:0169-3204-90	3 mL in 1 SYRINGE, PLASTIC; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		

Marketing Information

Marketing Category	Application Number or Monograph Citation	Marketing Start Date	Marketing End Date
BLA	BLA208751	10/20/2017	

FIASP

insulin aspart injection injection, solution

Product Information

Product Type	HUMAN PRESCRIPTION DRUG	Item Code (Source)	NDC:0169-3205
Route of Administration	SUBCUTANEOUS		

Active Ingredient/Active Moiety

Ingredient Name	Basis of Strength	Strength
INSULIN ASPART (UNII: D933668QVX) (INSULIN ASPART - UNII:D933668QVX)	INSULIN ASPART	100 [iU] in 1 mL

Inactive Ingredients

Ingredient Name	Strength
SODIUM PHOSPHATE, DIBASIC, UNSPECIFIED FORM (UNII: GR686LBA74)	0.42 mg in 1 mL
WATER (UNII: 059QF0KO0R)	

Other Ingredients

Ingredient Kind	Ingredient Name	Quantity
May contain	HYDROCHLORIC ACID (UNII: QTT17582CB)	
May contain	SODIUM HYDROXIDE (UNII: 55X04QC32I)	

Packaging				
#	Item Code	Package Description	Marketing Start Date	Marketing End Date
1	NDC:0169-3205-15	5 in 1 CARTON	10/01/2019	
1	NDC:0169-3205-11	3 mL in 1 CARTRIDGE; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		
2	NDC:0169-3205-95	5 in 1 CARTON	10/01/2019	
2	NDC:0169-3205-91	3 mL in 1 CARTRIDGE; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		

Marketing Information			
Marketing Category	Application Number or Monograph Citation	Marketing Start Date	Marketing End Date
BLA	BLA208751	10/20/2017	

FIASP				
insulin aspart injection, solution				
Product Information				
Product Type	HUMAN PRESCRIPTION DRUG	Item Code (Source)	NDC:0169-3206	
Route of Administration	SUBCUTANEOUS			
Active Ingredient/Active Moiety				
	Ingredient Name	Basis of Strength	Strength	
	INSULIN ASPART (UNII: D933668QVX) (INSULIN ASPART - UNII:D933668QVX)	INSULIN ASPART	100 [iU] in 1 mL	
Inactive Ingredients				
	Ingredient Name	Strength		
	WATER (UNII: 059QF0KO0R)			
Other Ingredients				
	Ingredient Kind	Ingredient Name	Quantity	
	May contain	HYDROCHLORIC ACID (UNII: QTT17582CB)		
	May contain	SODIUM HYDROXIDE (UNII: 55X04QC32I)		
Packaging				
#	Item Code	Package Description	Marketing Start Date	Marketing End Date
1	NDC:0169-3206-15	5 in 1 CARTON	09/14/2023	

1	NDC:0169-3206-11	1.6 mL in 1 CARTRIDGE; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		
2	NDC:0169-3206-95	5 in 1 CARTON	09/14/2023	
2	NDC:0169-3206-91	1.6 mL in 1 CARTRIDGE; Type 3: Prefilled Biologic Delivery Device/System (syringe, patch, etc.)		

Marketing Information

Marketing Category	Application Number or Monograph Citation	Marketing Start Date	Marketing End Date
BLA	BLA208751	10/20/2017	

Labeler - Novo Nordisk (622920320)

Revised: 6/2023

Novo Nordisk