

## OXYGEN- oxygen gas Sparrow Medical Supply L.L.C.

*Disclaimer: This drug has not been found by FDA to be safe and effective, and this labeling has not been approved by FDA. For further information about unapproved drugs, click here.*

### Labels

#### Oxygen Label 1



**WARNING:** For emergency use only when administered by properly trained personnel for oxygen deficiency or resuscitation in case of medical and dental emergencies. Do NOT USE compressed gas for non-medical purposes. Oxygen can burn with explosive violence, without warning, in heat or oxygen converter. Should never may mix with oil. Do not store open or use equipment and have storage involving a heat source in any normal use, resuscitation equipment.

**WARNING: HIGH PRESSURE OXIDIZING GAS  
VIGOROUSLY ACCELERATES COMBUSTION**

- Do not use compressed gas equipment in hospitals, dental and medical facilities.
- Open valve slowly. Close valve slowly when use and when empty. Stop cylinder, cylinder valve, and valve stem assembly, two cr all use grease to avoid violent ignition.
- Never allow any part of the cylinder to be heated with oxygen. Use only by calculations required as a temperature indicator in cooperation with the United States Drug and Cosmetic Commission.
- Follow recommendations by Commercial Gas Association. do not expose gas to temperatures in excess of 125°F.
- DO NOT RE-ROUTE CYLINDER VALVE.  
Use only in accordance with printed instructions and caution safety data sheet.

Rev. date: 10/03

2000-0005-2000

Distributed by:

**SPARROW**  
REGIONAL  
MEDICAL SUPPLY

915 East Michigan Avenue  
Lansing, MI 48912

(877) 205-3500  
(517) 364-2115

**WARNING:**

**HIGH PRESSURE GAS CYLINDER**

Important: If you abuse of this cylinder, in the event of fire, the warping may cause severe injury to the user. Do NOT ALTER OR MODIFY CYLINDER OR BELTING COMPONENTS. DO NOT OVER PRESSURIZE. Keep out of the reach of children. Cylinders that have been overheated and/or exposed to intense temperatures, such as hydrocarbons, acids, sulfuric acid, etc., or hot caustic metal vapors. Aluminum cylinders subject to action of fire or heated to temperatures in excess of 500°F must be off service from service and condemned. Values and safety relief valves must be examined and tested to make sure that the cylinder is strong, safety discs, replace broken relief discs only with original assemblies supplied by the valve manufacturer. DO NOT USE WITH OXIDIZING AGENTS. WASHOUT. PROPER CLEANING: Cylinder valves and associated parts must be cleaned after oxygen. Verify cylinder contents and pressure monthly, or more frequently if required. Store and use with adequate ventilation.

**Cylinder contents at 70°F**

Type

O A	-	113 liters at 2216 PSI
O B	-	164 liters at 2216 PSI
O C	-	248 liters at 2015 PSI
O D	-	414 liters at 2015 PSI
O E	-	682 liters at 2015 PSI
O Q	-	1723 liters at 2216 PSI

#### Oxygen label 2



**UN1073**

**WARNING!**

Extremely cold liquid and gas under pressure. Vigorously accelerates combustion.

PRODUCED BY AIR LIQUEFACTION



CYLINDER FILLED BY

**SPARROW**  
REGIONAL  
MEDICAL SUPPLY

915 East Michigan Avenue  
Lansing, MI 48912

(877) 205-3500  
(517) 364-2115

**Warning!**

For emergency use only when administered by properly trained personnel for oxygen deficiency and resuscitation. Can cause extreme frost bite.

**Keep Out of Reach of Children.**

Contents under pressure and can vigorously accelerate combustion. Keep free from oil and grease. Do not use or store near heat or open flame and use only with equipment conditioned for oxygen service. Open valve slowly. Close valve when not in use and when empty. Store and use with adequate ventilation to prevent oxygen accumulation.

LOT#, \_\_\_\_\_ EXP. \_\_\_\_\_ LITERS \_\_\_\_\_

**Caution:** Federal law prohibits dispensing without prescription. For non-medical applications, use only as directed by a licensed practitioner. Uninterrupted use of high concentrations of oxygen for more than 8 hours, may be harmful. Use only with pressure reducing equipment and apparatus designed for oxygen.

Federal law requires that this cylinder be refilled with Oxygen, U.S.P. only by establishments registered as a drug producer in accordance with the Federal Food, Drug and Cosmetic Act.

**DO NOT REMOVE THIS LABEL**

#### Oxygen Label 3

## Oxygen, Refrigerated Liquid U.S.P.

### WARNING!

DO NOT CHANGE OR FORCE FIT CONNECTIONS. EXTREMELY COLD OXIDIZING LIQUID AND GAS UNDER PRESSURE VIGOROUSLY ACCELERATES COMBUSTION. NO SMOKING IN THE PRESENCE OF OXYGEN OR A FIRE MAY RESULT. COMBUSTIBLES IN CONTACT WITH LIQUID OXYGEN MAY EXPLODE ON IGNITION OR IMPACT. CAN CAUSE SEVERE FROSTBITE.



CYLINDER FILLED BY

**SPARROW**

REGIONAL  
MEDICAL SUPPLY

915 East Michigan Avenue  
Lansing, MI 48912

(877) 205-3500  
(517) 364-2115

### WARNING!

Keep oil, grease, and combustibles away. Use only with equipment cleaned for oxygen service. Store and use with adequate ventilation. Do not get liquid in eyes, on skin or clothing. For liquid withdrawal, wear face shield and gloves. Do not drip. Use suitable hand truck for container movement. Avoid spills. Do not walk on or roll equipment over spills. Container temperature should not exceed 62°C (125°F). Close valve after each use and when empty. Use a back flow preventer device in the piping. Use in accordance with the Material Safety Data Sheet (MSDS). FIRST AID: IN CASE OF FROSTBITE, obtain medical treatment immediately.

### WARNING:

For emergency use only when administered by properly trained personnel for oxygen deficiency and resuscitation. For all other medical applications, Rx Only. Uninterrupted use of high concentrations of oxygen over a long duration, without monitoring its effect on oxygen content of arterial blood, may be harmful. Use only with pressure reducing equipment and apparatus designed for oxygen. Do not attempt to use on patients who have stopped breathing, unless used in conjunction with resuscitative equipment. Produced by Air Liquification.

Contents: \_\_\_\_\_ liters

**DO NOT REMOVE THIS LABEL.**

## Oxygen Label 4

Produced by air liquification

**OXYGEN  
COMPRESSED  
U.S.P. UN 1072**



**WARNING:** For emergency use only when administered by properly trained personnel for oxygen deficiency and resuscitation. For all other medical applications, Rx Only. Uninterrupted use of high concentrations of oxygen over a long duration, without monitoring its effect on oxygen content of arterial blood, may be harmful. Do not attempt to use on patients who have stopped breathing unless used in conjunction with resuscitative equipment.

### WARNING: HIGH PRESSURE OXIDIZING GAS VIGOROUSLY ACCELERATES COMBUSTION

- Use only with pressure reducing equipment and apparatus cleaned and designed for oxygen service and rated for cylinder pressure.
- Open valve slowly. Close valve after each use and when empty. Keep cylinder, cylinder valve, all equipment that connects, free of oil and grease to avoid violent ignition.
- Federal law requires that this container be refilled with oxygen USP only by establishments registered as a drug manufacturer in accordance with the Federal Food, Drug and Cosmetic Act.
- Pursuant to recommendations by Compressed Gas Association, do not expose pressurized cylinders to temperatures in excess of 125°F.
- **DO NOT REMOVE THIS PRODUCT LABEL.**

Use only in accordance with product instructions and material safety data sheet.

Date code: 1992

Distributed by:

**Sparrow**  
Medical Supply

915 East Michigan Avenue  
Lansing, MI 48912

(877) 205-3500  
(517) 364-2115

### WARNING:

**HIGH PRESSURE GAS CYLINDER**  
Improper filling or abuse of this cylinder, or failure to heed this warning may cause serious injury or loss of life. **DO NOT ALTER OR MODIFY CYLINDER OR RELATED COMPONENTS. DO NOT OVERPRESSURIZE.** Keep out of the reach of children. Cylinders that have been refilled and/or exposed to elevated temperatures must be hydrostatically tested before filling. Do not use caustic paint strippers. Aluminum cylinders subject to action of fire or heated to temperatures in excess of 350°F must be withdrawn from service and condemned. Valves and safety relief devices must be removed and replaced by trained personnel. Do not alter or change safety discs. Replace pressure relief devices only with complete assemblies supplied by the valve manufacturer. **DO NOT FILL WITH OXIDIZING GASES WITHOUT PROPER CLEANING.** Cylinders, valves, and assemblies must be specially cleaned for oxygen. Verify cylinder content and pressure monthly, or more frequently if required. Store and use with adequate ventilation.

### Cylinder contents at 70°F

Type	
O A	- 113 liters at 2216 PSI
O B	- 164 liters at 2216 PSI
O C	- 248 liters at 2015 PSI
O D	- 414 liters at 2015 PSI
O E	- 682 liters at 2015 PSI
O Q	- 1723 liters at 2216 PSI

## Oxygen Label 5

# Oxygen, Refrigerated Liquid U.S.P.

## WARNING!



DO NOT CHANGE OR FORCE FIT CONNECTIONS, EXTREMELY COLD OXIDIZING LIQUID AND GAS UNDER PRESSURE VIGOROUSLY ACCELERATES COMBUSTION. NO SMOKING IN THE PRESENCE OF OXYGEN OR A FIRE MAY RESULT. COMBUSTIBLES IN CONTACT WITH LIQUID OXYGEN MAY EXPLODE ON IGNITION OR IMPACT. CAN CAUSE SEVERE FROSTBITE.

## WARNING:

For emergency use only when administered by properly trained personnel for oxygen deficiency and resuscitation. For all other medical applications, Rx Only. Uninterrupted use of high concentrations of oxygen over a long duration, without monitoring its effect on oxygen content of arterial blood, may be harmful. Use only with pressure reducing equipment and apparatus designed for oxygen. Do not attempt to use on patients who have stopped breathing, unless used in conjunction with resuscitative equipment. Produced by Air Liquification.

Contents: \_\_\_\_\_ LITERS

CYLINDER FILLED BY

Sparrow  
Medical Supply

915 East Michigan Avenue  
Lansing, MI 48912

(877) 205-3500  
(517) 364-2115

## WARNING!

Keep oil, grease, and combustibles away. Use only with equipment cleaned for oxygen service. Store and use with adequate ventilation. Do not get liquid in eyes, on skin or clothing. For liquid withdrawal, wear face shield and gloves. Do not drip. Use suitable hand truck for container movement. Avoid spills. Do not walk on or roll equipment over spills. Container temperature should not exceed 52°C (125°F). Close valve after each use and when empty. Use a back flow preventative device in the piping. Use in accordance with the Material Safety Data Sheet (MSDS).


FIRST AID:  
IN CASE OF FROSTBITE, obtain medical treatment immediately.

DO NOT REMOVE THIS LABEL

## Oxygen Label 6

Produced by air liquefaction

OXYGEN  
COMPRESSED  
U.S.P. UN 1072  
**DANGER**



Distributed by:  
 Sparrow  
Medical Supply

915 East Michigan Avenue  
Lansing, MI 48912

(877) 205-3500  
(517) 364-2115

## WARNING:

**HIGH PRESSURE GAS CYLINDER**  
Improper filling or abuse of this cylinder, or failure to heed this warning may cause serious injury or loss of life. DO NOT ALTER OR MODIFY CYLINDER OR RELATED COMPONENTS. DO NOT OVER PRESSURIZE. Keep out of the reach of children. Cylinders that have been refinished and/or exposed to elevated temperatures must be hydrostatically tested before filling. Do not use caustic paint strippers. Aluminum cylinders subject to action of fire or heated to temperatures in excess of 350°F must be withdrawn from service and condemned. Valves and safety relief devices must be removed and replaced by trained personnel. Do not alter or change safety discs. Replace pressure relief devices only with complete assemblies supplied by the valve manufacturer. DO NOT FILL WITH OXIDIZING GASES WITHOUT PROPER CLEANING. Cylinders, valves, and assemblies must be specially cleaned for oxygen. Verify cylinder content and pressure monthly, or more frequently if required. Store and use with adequate ventilation.

### Cylinder contents at 70°F

#### Type


<input type="radio"/>	A	-	113 liters at 2216 PSI
<input type="radio"/>	B	-	164 liters at 2216 PSI
<input type="radio"/>	C	-	248 liters at 2015 PSI
<input type="radio"/>	D	-	414 liters at 2015 PSI
<input type="radio"/>	E	-	682 liters at 2015 PSI
<input type="radio"/>	Q	-	1723 liters at 2216 PSI

## Oxygen Label 7

**DANGER**



## Oxygen Label 8

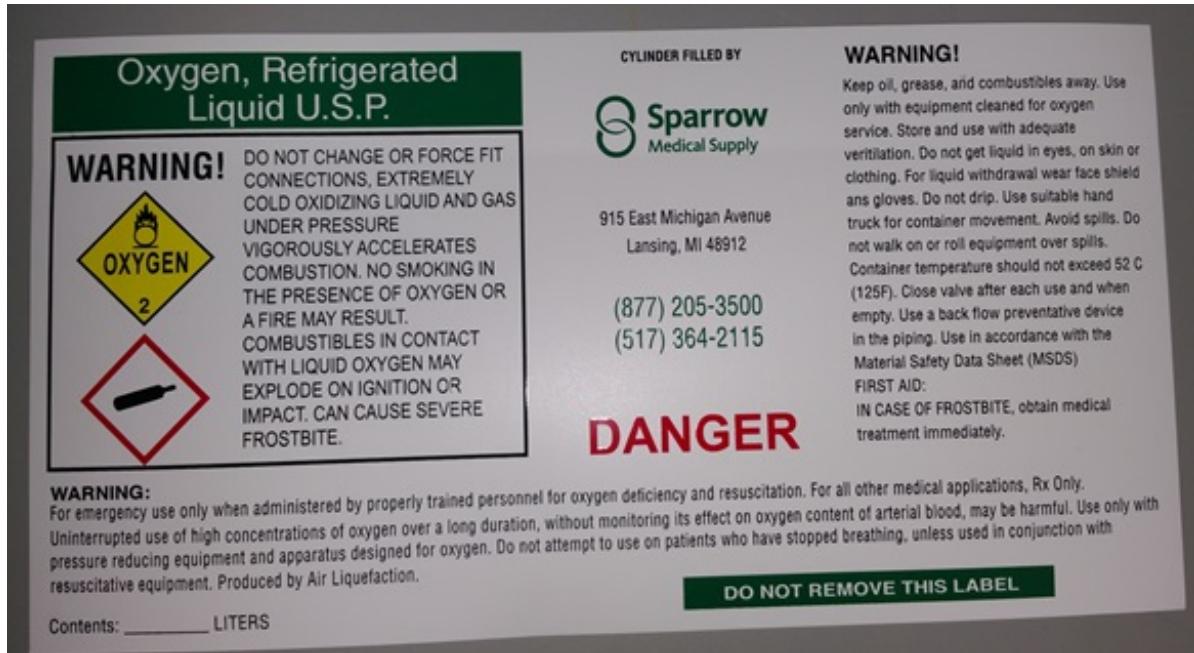

## OXYGEN

oxygen gas

### Product Information

<b>Product Type</b>	HUMAN PRESCRIPTION DRUG	<b>Item Code (Source)</b>	NDC:54595-001
<b>Route of Administration</b>	RESPIRATORY (INHALATION)		

### Active Ingredient/Active Moiety

Ingredient Name	Basis of Strength	Strength
OXYGEN (UNII: S88TT14065) (OXYGEN - UNII:S88TT14065)	OXYGEN	99 mL in 1 L

### Packaging

#	Item Code	Package Description	Marketing Start Date	Marketing End Date
1	NDC:54595-001-50	248 L in 1 CYLINDER; Type 0: Not a Combination Product	12/05/1994	
2	NDC:54595-001-40	164 L in 1 CYLINDER; Type 0: Not a Combination Product	12/05/1994	
3	NDC:54595-001-60	414 L in 1 CYLINDER; Type 0: Not a Combination Product	12/05/1994	
4	NDC:54595-001-70	682 L in 1 CYLINDER; Type 0: Not a Combination Product	12/05/1994	
5	NDC:54595-001-90	184 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	
6	NDC:54595-001-30	113 L in 1 CYLINDER; Type 0: Not a Combination Product	12/05/1994	
7	NDC:54595-001-80	1723 L in 1 CYLINDER; Type 0: Not a Combination Product	12/05/1994	
8	NDC:54595-001-91	7749 L in 1 CYLINDER; Type 0: Not a Combination Product	12/05/1994	
9	NDC:54595-001-10	46 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	
10	NDC:54595-001-20	30 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	

11	NDC:54595-001-21	46 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	
12	NDC:54595-001-22	36 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	
13	NDC:54595-001-23	10 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	
14	NDC:54595-001-24	720 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	
15	NDC:54595-001-25	225 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	
16	NDC:54595-001-26	451 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	
17	NDC:54595-001-27	277 L in 1 DEWAR; Type 0: Not a Combination Product	12/05/1994	

## Marketing Information

Marketing Category	Application Number or Monograph Citation	Marketing Start Date	Marketing End Date
unapproved medical gas		07/01/1994	

**Labeler** - Sparrow Medical Supply L.L.C. (837040336)

**Registrant** - Sparrow Medical Supply L.L.C. (837040336)

## Establishment

Name	Address	ID/FEI	Business Operations
Sparrow Medical Supply L.L.C.		837040336	manufacture(54595-001)

Revised: 10/2020

Sparrow Medical Supply L.L.C.