

**TD GOLD VOICE BLOOD GLUCOSE MONITOR SET- glucose oxidase, glucose
EPS Bio Technology Corp.**

Home Use Medical Device : TD Gold Voice Self-monitoing Blood Glucose System

TD Gold Voice Blood Glucose Monitor Box

55T 安娜白卡
153x90x44mm

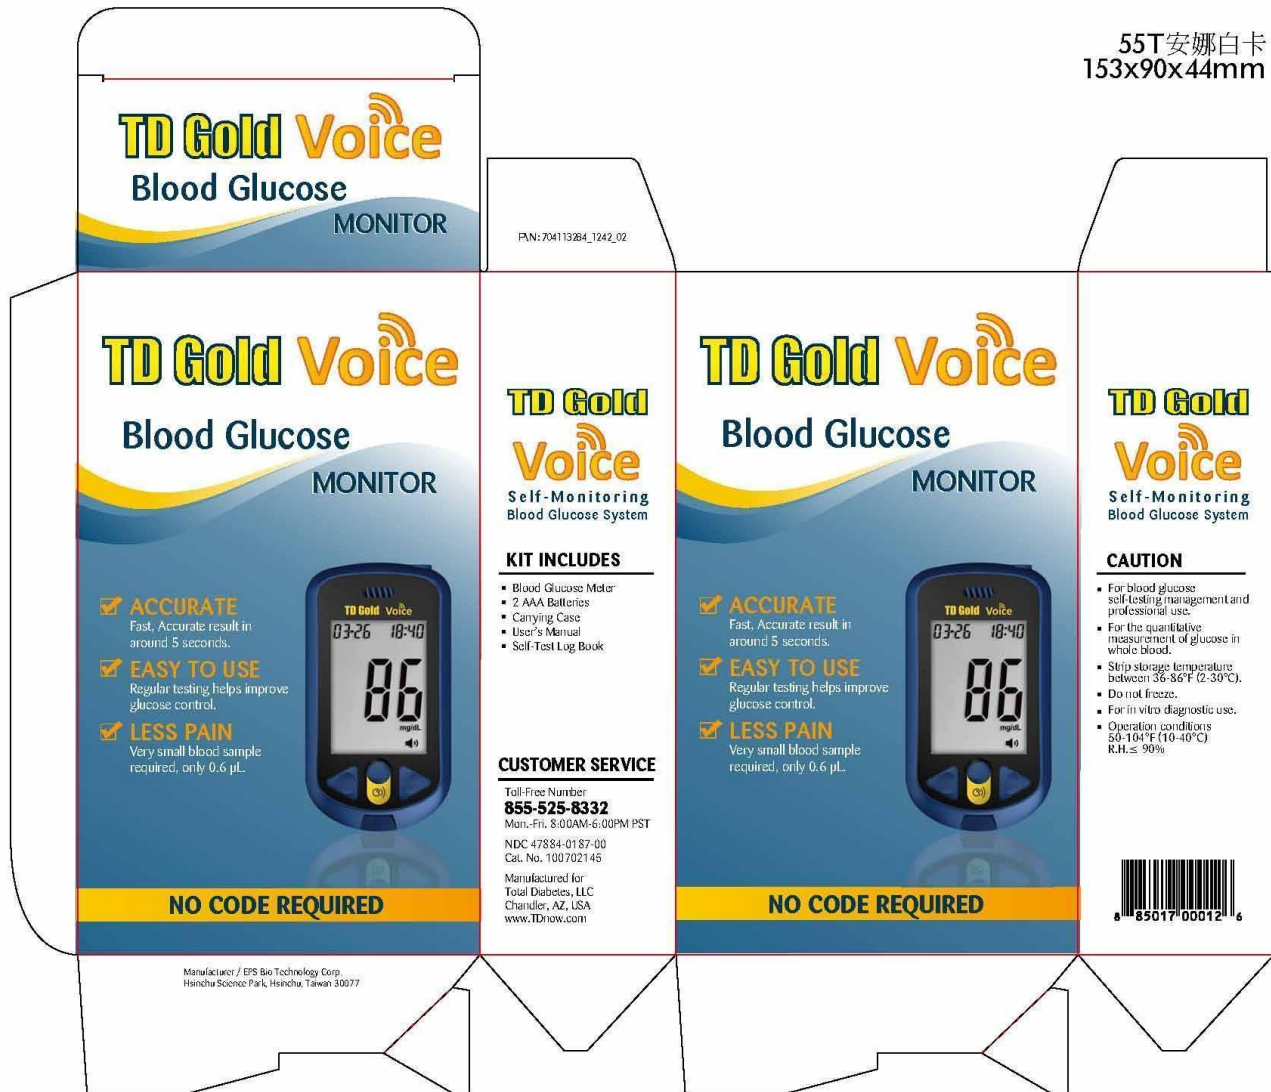


Diagram of TD Gold Voice Blood Glucose Meter

1	PE Film BIV	70004000	I-S-02404
2	Wear Plate BIV-III	700040100	I-S-02564
3	Double Tape 2041	700040300	I-S-02560
4	SPRING 204	702002300	I-S-02113
5	Front Cover EMV-III	700040200	I-S-02565
6	Carriage Lubric Part BIV-III	700040400	I-S-02567
7	PSD-508 PCLA	700040300	NA
8	Battery Pkg (2Pcs)	702001700	I-S-02062
9	Back Cover BIV-III	700040300	I-S-02568
10	Spring C (2Pcs)	702001600	I-S-02380
11	Spring A (2Pcs)	702001400	I-S-02024
12	Spring B (2Pcs)	702001500	I-S-02060
13	Battery Cover BIV-III	700040200	I-S-02568
14	Holder Stand T2	700001300	I-S-02087
15	BIV Power Label 2	704001700	I-S-02048

1.	New Design	200807
Rev	Revising Statement	Date

1. UNLESS OTHERWISE SPECIFIED
2. DIMENSIONS ARE IN MILLIMETERS
3. TOLERANCES: DECIMALS: >0.03 - ±0.05 ANGULAR: >10° - ±0.1° >100° - ±0.5° >1000° - ±1.2°
4.50-90° SCALE DRAWING

EPS Bio Technology Corp.

TITLE: Meter ASSY EMV-III

SIZE (A4) DWG. NO. I-D-CO-0000 A

SCALE 1X SHEET 1 OF 1

TD GOLD VOICE BLOOD GLUCOSE MONITOR SET

glucose oxidase, glucose

Product Information

Product Type	MEDICAL DEVICE	Item Code (Source)	NHRIC:47884-187
--------------	----------------	--------------------	-----------------

Product Characteristics

number of times usable	10000
------------------------	-------

Packaging

#	Item Code	Package Description	Marketing Start Date	Marketing End Date
1	NHRIC:47884-187-00	1 in 1 KIT		

Marketing Information

Marketing Category	Application Number or Monograph Citation	Marketing Start Date	Marketing End Date
premarket notification	K111728	10/01/2013	

Labeler - EPS Bio Technology Corp. (658620117)

Revised: 10/2013

EPS Bio Technology Corp.